

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102124\
 Data File : VW030685.D
 Acq On : 21 Oct 2024 17:13
 Operator : SY/MD
 Sample : P4415-13
 Misc : 3.48g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 22 01:36:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Oct 22 01:33:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.849	114	3138	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.629	117	3232	25.000	ug/L	# 0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	1053	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	723	14.658	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	58.640%
7) Chloroethane-d5	2.905	69	889	23.810	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.240%
11) 1,1-Dichloroethene-d2	4.015	65	140	6.824	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	27.280%#
21) 2-Butanone-d5	7.075	46	97	10.928	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	21.860%
24) Chloroform-d	7.654	84	2931	32.661	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	130.640%
26) 1,2-Dichloroethane-d4	8.307	65	2215	47.466	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	189.880%#
32) Benzene-d6	8.276	84	3517	18.749	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	75.000%
36) 1,2-Dichloropropane-d6	9.276	67	1822	33.092	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	132.360%#
41) Toluene-d8	10.331	98	2014	11.761	ug/L	0.01
Spiked Amount	25.000	Range	30 - 130	Recovery	=	47.040%
43) trans-1,3-Dichloroprop...	10.587	79	441	19.128	ug/L	0.01
Spiked Amount	25.000	Range	30 - 135	Recovery	=	76.520%
47) 2-Hexanone-d5	10.953	63	166	23.409	ug/L	0.03
Spiked Amount	50.000	Range	20 - 135	Recovery	=	46.820%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	2016	49.859	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	199.440%#
66) 1,2-Dichlorobenzene-d4	13.855	152	991	27.814	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	111.240%
Target Compounds						
					Qvalue	
3) Chloromethane	2.265	50	248	5.322	ug/L	88
6) Bromomethane	2.716	94	78	2.068	ug/L	# 5
8) Chloroethane	2.917	64	80	2.284	ug/L	# 56
9) Trichlorofluoromethane	3.259	101	68	1.326	ug/L	# 18
12) 1,1-Dichloroethene	3.850	96	41	0.974	ug/L	# 1
13) Acetone	4.137	43	1405	108.114	ug/L	80
15) Methyl Acetate	4.673	43	23	1.433	ug/L	# 51
17) trans-1,2-Dichloroethene	5.472	96	81	1.783	ug/L	# 1
19) 1,1-Dichloroethane	6.173	63	86	1.019	ug/L	# 49
22) 2-Butanone	7.215	43	70	4.997	ug/L	95
25) Chloroform	7.526	83	45	0.499	ug/L	# 18
27) 1,2-Dichloroethane	8.410	62	38	0.638	ug/L	# 76
29) Cyclohexane	7.996	56	47	0.597	ug/L	# 11
30) 1,1,1-Trichloroethane	7.941	97	48	0.559	ug/L	# 8
34) Trichloroethene	8.843	95	28	0.479	ug/L	# 5
35) Methylcyclohexane	9.331	83	90	0.977	ug/L	# 17
37) 1,2-Dichloropropane	9.386	63	42	0.800	ug/L	# 86
39) cis-1,3-Dichloropropene	10.142	75	48	0.606	ug/L	# 1
40) 4-Methyl-2-pentanone	10.221	43	46	1.823	ug/L	# 43

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102124\
 Data File : VW030685.D
 Acq On : 21 Oct 2024 17:13
 Operator : SY/MD
 Sample : P4415-13
 Misc : 3.48g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 22 01:36:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Oct 22 01:33:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


42) Toluene	10.392	91	249	1.110	ug/L	80
44) trans-1,3-Dichloropropene	10.617	75	65	0.976	ug/L #	1
45) 1,1,2-Trichloroethane	10.660	97	122	3.214	ug/L #	16
49) Dibromochloromethane	11.032	129	73	1.723	ug/L #	9
53) m,p-Xylene	11.733	106	49	0.511	ug/L #	17
54) o-Xylene	12.306	106	43	0.485	ug/L #	1
55) Styrene	11.983	104	57	0.376	ug/L #	28
57) 1,1,2,2-Tetrachloroethane	12.751	83	21	0.491	ug/L #	27
61) 1,2,3-Trichloropropane	12.775	75	54	2.635	ug/L #	28
63) 1,2,4-Trimethylbenzene	13.227	105	48	0.381	ug/L #	31
64) 1,3-Dichlorobenzene	13.574	146	45	0.634	ug/L #	23
65) 1,4-Dichlorobenzene	13.574	146	45	0.614	ug/L #	28
67) 1,2-Dichlorobenzene	14.111	146	43	0.688	ug/L #	23
71) Naphthalene	15.458	128	51	0.783	ug/L #	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102124\
Data File : VW030685.D
Acq On : 21 Oct 2024 17:13
Operator : SY/MD
Sample : P4415-13
Misc : 3.48g/10mL/MSVOA_W/SOIL/A
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Oct 22 01:36:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Oct 22 01:33:40 2024
Response via : Initial Calibration




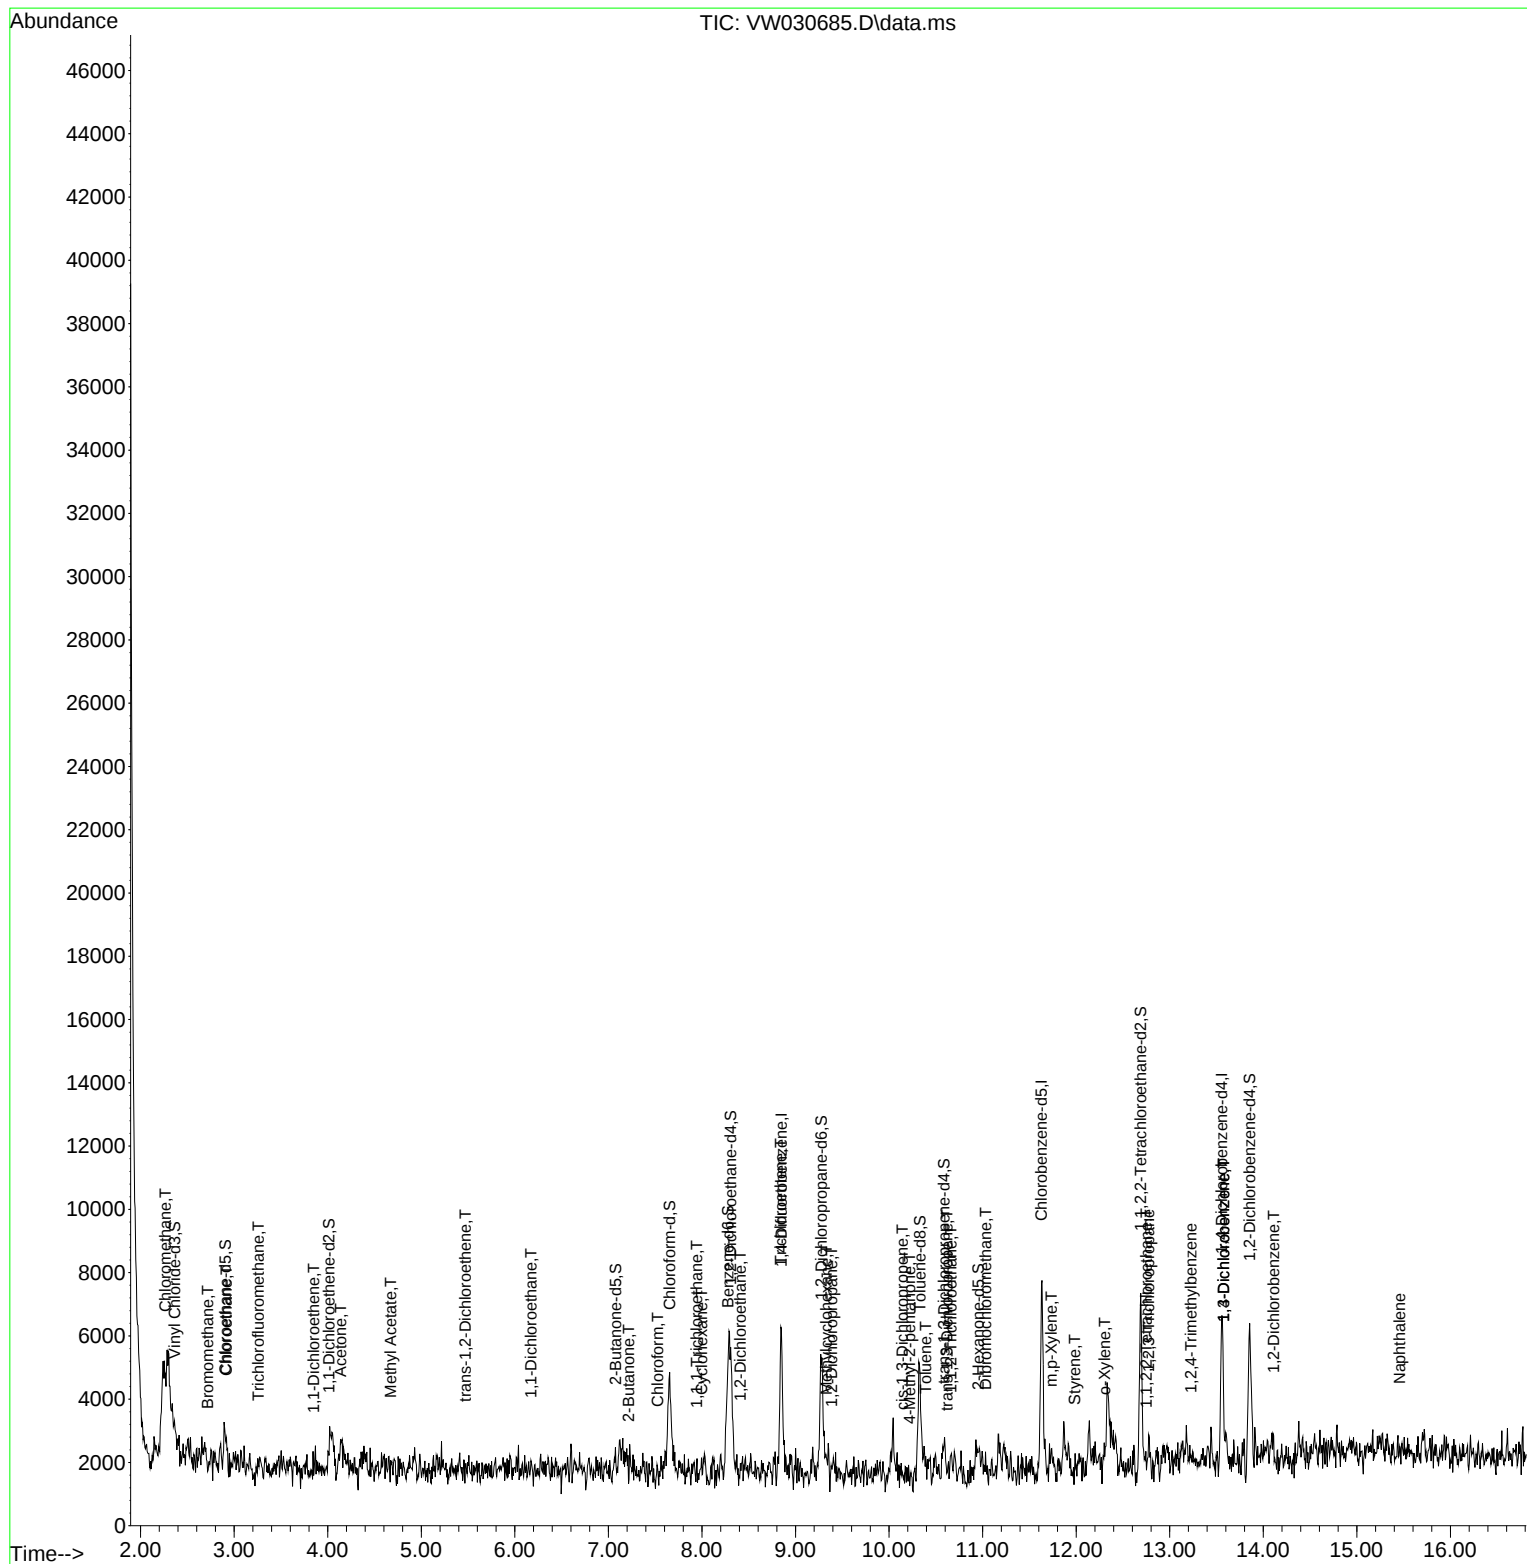




#3
Chloromethane
Concen: 5.322 ug/L
RT: 2.265 min Scan# 61
Delta R.T. 0.043 min
Lab File: VW030685.D
Acq: 21 Oct 2024 17:13




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 50 Resp: 248
Ion Ratio Lower Upper
50 100
52 40.6 23.7 43.9

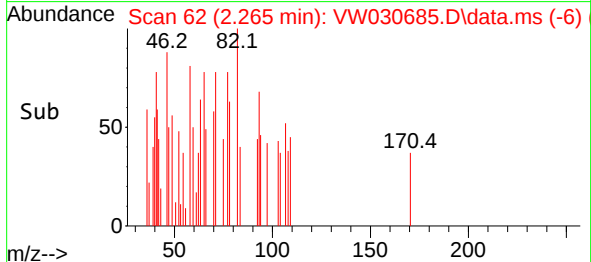

#6
Bromomethane
Concen: 2.068 ug/L
RT: 2.716 min Scan# 136
Delta R.T. -0.073 min
Lab File: VW030685.D
Acq: 21 Oct 2024 17:13

Tgt Ion: 94 Resp: 78
Ion Ratio Lower Upper
94 100
96 0.0 62.6 116.2#


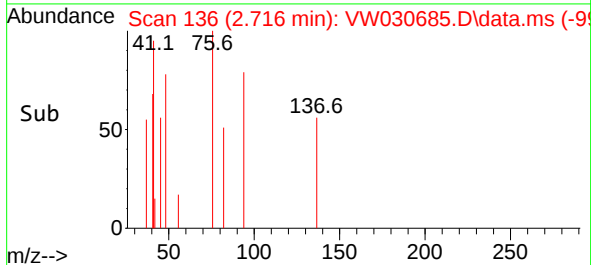

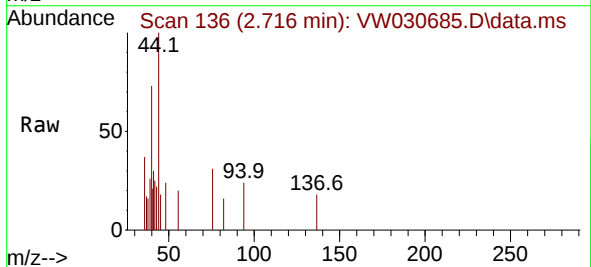




#8
Chloroethane
Concen: 2.284 ug/L
RT: 2.917 min Scan# 110
Delta R.T. -0.018 min
Lab File: VW030685.D
Acq: 21 Oct 2024 17:13




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 64 Resp: 80
Ion Ratio Lower Upper
64 100
66 56.3 22.3 41.5#

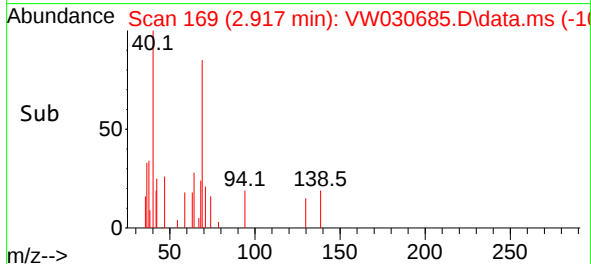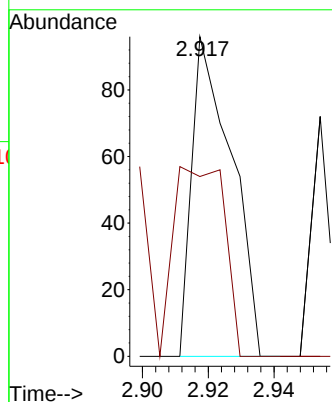

#9
Trichlorofluoromethane
Concen: 1.326 ug/L
RT: 3.259 min Scan# 225
Delta R.T. -0.006 min
Lab File: VW030685.D
Acq: 21 Oct 2024 17:13

Tgt Ion: 101 Resp: 68
Ion Ratio Lower Upper
101 100
103 0.0 51.1 76.7#


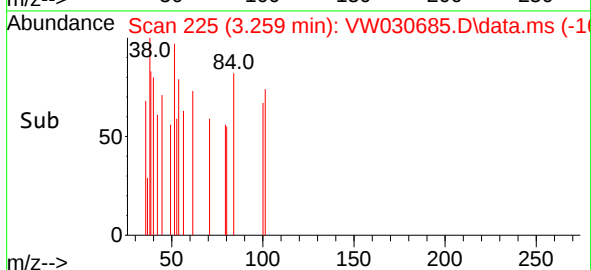






#12
1,1-Dichloroethene
Concen: 0.974 ug/L
RT: 3.850 min Scan# 31
Delta R.T. -0.189 min
Lab File: VW030685.D
Acq: 21 Oct 2024 17:13




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 96 Resp: 41
Ion Ratio Lower Upper
96 100
61 0.0 121.3 225.3#
63 0.0 87.6 162.8#

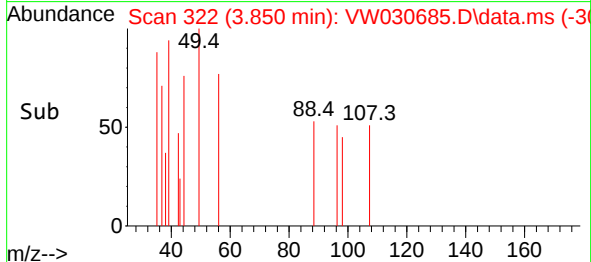

#13
Acetone
Concen: 108.114 ug/L
RT: 4.137 min Scan# 369
Delta R.T. 0.012 min
Lab File: VW030685.D
Acq: 21 Oct 2024 17:13

Tgt Ion: 43 Resp: 1405
Ion Ratio Lower Upper
43 100
58 18.4 0.0 57.6


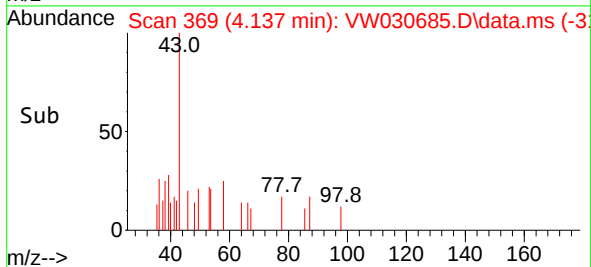

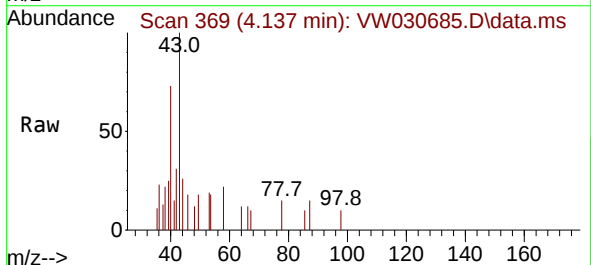




#15
Methyl Acetate
Concen: 1.433 ug/L
RT: 4.673 min Scan# 41
Delta R.T. 0.000 min
Lab File: VW030685.D
Acq: 21 Oct 2024 17:13




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 43 Resp: 23
Ion Ratio Lower Upper
43 100
74 0.0 19.3 28.9#

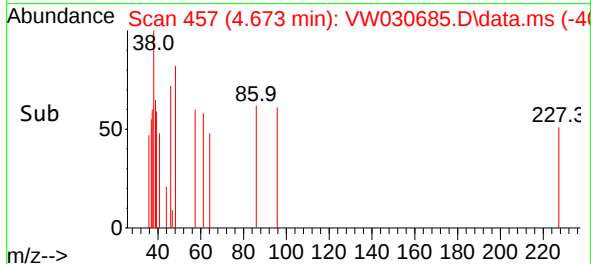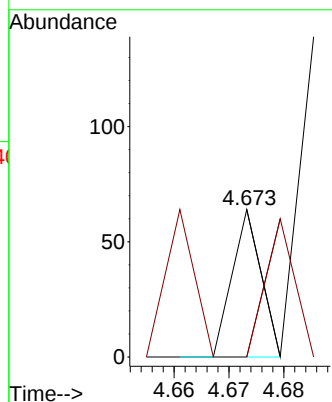

#17
trans-1,2-Dichloroethene
Concen: 1.783 ug/L
RT: 5.472 min Scan# 588
Delta R.T. 0.043 min
Lab File: VW030685.D
Acq: 21 Oct 2024 17:13

Tgt Ion: 96 Resp: 81
Ion Ratio Lower Upper
96 100
61 0.0 96.9 179.9#
98 0.0 42.2 78.4#

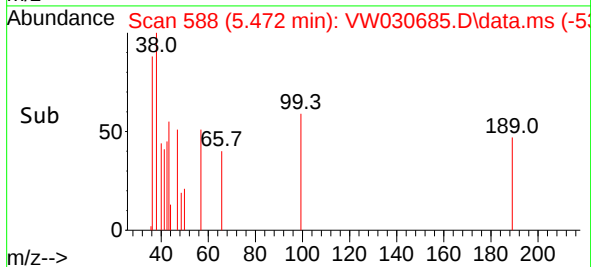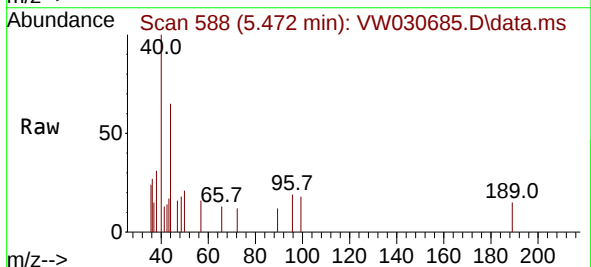



#19

1,1-Dichloroethane

Concen: 1.019 ug/L

RT: 6.173 min Scan# 709

Delta R.T. -0.037 min

Lab File: VW030685.D





Acq: 21 Oct 2024 17:13

Instrument :

MSVOA_W

ClientSampleId :

Tgt Ion:	63	Resp:	86
Ion	Ratio	Lower	Upper
63	100		
65	0.0	22.5	41.9#
83	0.0	9.8	18.2#

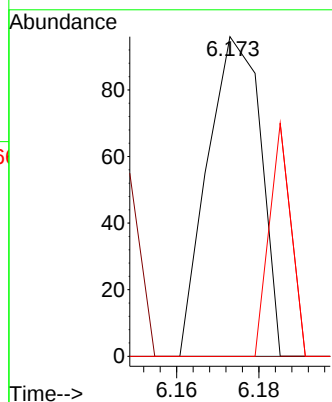

#22

2-Butanone

Concen: 4.997 ug/L




RT: 7.215 min Scan# 874


Delta R.T. 0.049 min

Lab File: VW030685.D

Acq: 21 Oct 2024 17:13

Tgt Ion:	43	Resp:	70
Ion	Ratio	Lower	Upper
43	100		
72	31.4	14.4	43.0


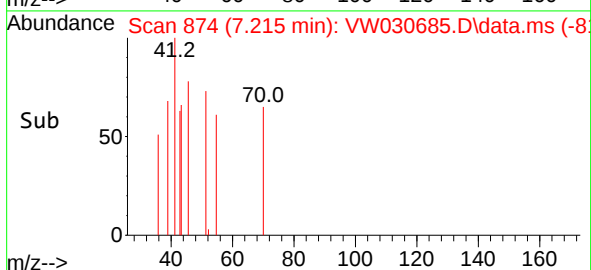






#25
Chloroform
Concen: 0.499 ug/L
RT: 7.526 min Scan# 91
Delta R.T. -0.146 min
Lab File: VW030685.D
Acq: 21 Oct 2024 17:13




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 83 Resp: 45
Ion Ratio Lower Upper
83 100
85 0.0 45.1 83.7#

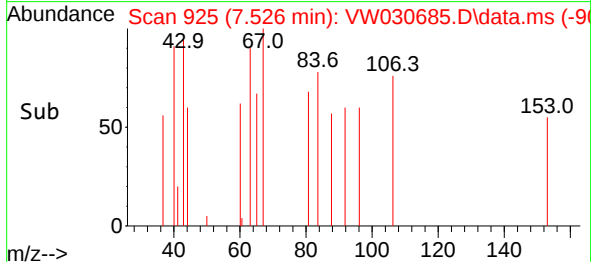

#27
1,2-Dichloroethane
Concen: 0.638 ug/L
RT: 8.410 min Scan# 1070
Delta R.T. 0.012 min
Lab File: VW030685.D
Acq: 21 Oct 2024 17:13

Tgt Ion: 62 Resp: 38
Ion Ratio Lower Upper
62 100
98 0.0 7.0 10.6#

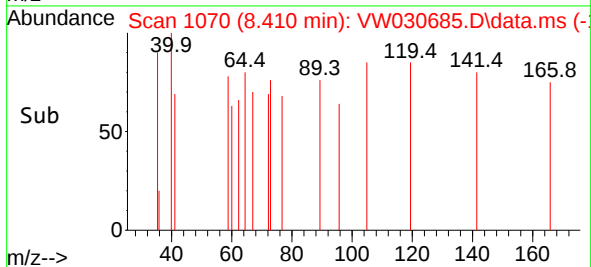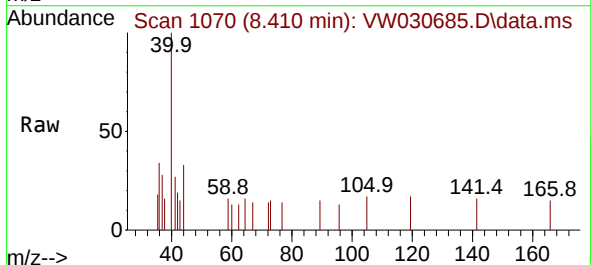



#29

Cyclohexane

Concen: 0.597 ug/L

RT: 7.996 min Scan# 1002

Delta R.T. 0.037 min

Lab File: VW030685.D

Acq: 21 Oct 2024 17:13

Instrument :

MSVOA_W

ClientSampleId :





Tgt Ion: 56 Resp: 47

Ion Ratio Lower Upper

56 100

69 0.0 25.4 38.0#

84 185.1 72.3 108.5#

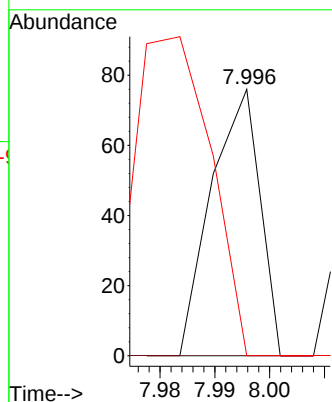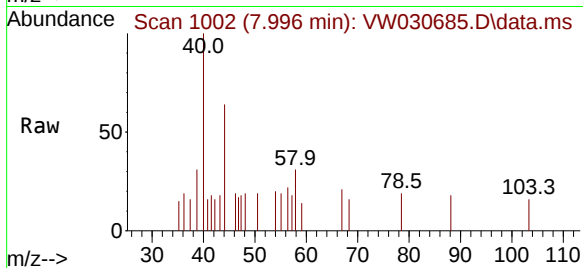

#30

1,1,1-Trichloroethane

Concen: 0.559 ug/L

RT: 7.941 min Scan# 993

Delta R.T. 0.073 min

Lab File: VW030685.D

Acq: 21 Oct 2024 17:13




Tgt Ion: 97 Resp: 48


Ion Ratio Lower Upper

97 100

99 0.0 52.3 78.5#

61 118.8 38.5 57.7#

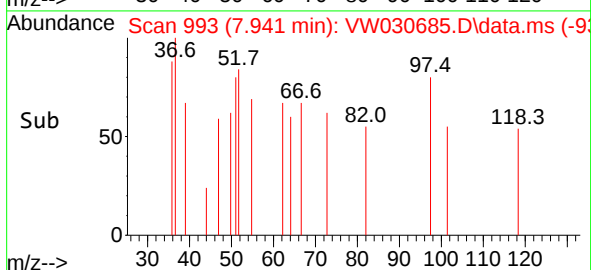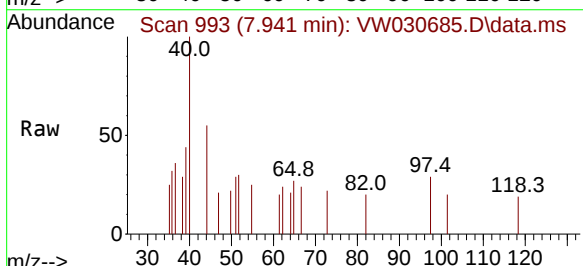

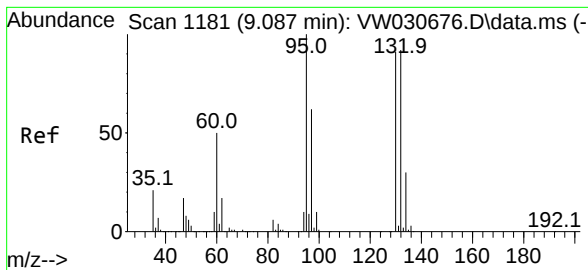

#34

Trichloroethene

Concen: 0.479 ug/L

RT: 8.843 min Scan# 1141

Delta R.T. -0.244 min


Lab File: VW030685.D

Acq: 21 Oct 2024 17:13

Instrument :

MSVOA_W

ClientSampleId :

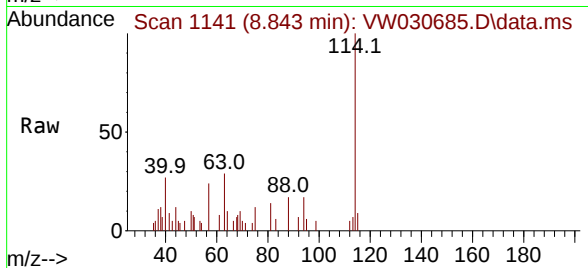

Tgt Ion: 95 Resp: 28




Ion Ratio Lower Upper

95 100

97 0.0 45.9 85.3#

132 0.0 66.4 123.2#

130 0.0 70.4 130.8#

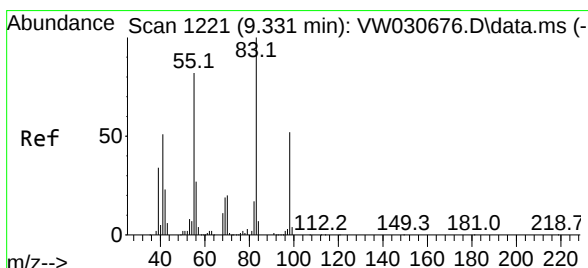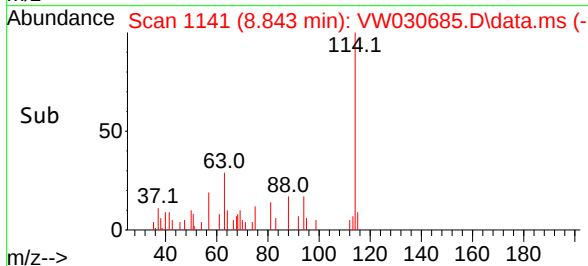

#35

Methylcyclohexane

Concen: 0.977 ug/L

RT: 9.331 min Scan# 1221

Delta R.T. 0.000 min

Lab File: VW030685.D

Acq: 21 Oct 2024 17:13




Tgt Ion: 83 Resp: 90


Ion Ratio Lower Upper

83 100

55 0.0 61.8 92.8#

98 0.0 39.3 58.9#

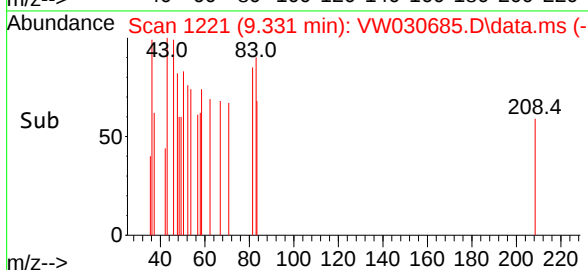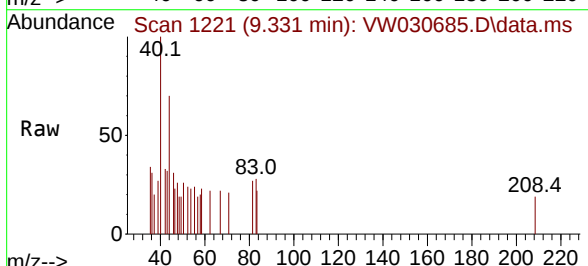



#37

1,2-Dichloropropane

Concen: 0.800 ug/L

RT: 9.386 min Scan# 11

Delta R.T. 0.018 min

Lab File: VW030685.D

Acq: 21 Oct 2024 17:13

Instrument :

MSVOA_W





ClientSampleId :

Tgt Ion: 63 Resp: 42

Ion Ratio Lower Upper

63 100

112 0.0 3.7 5.5#



#39

cis-1,3-Dichloropropene

Concen: 0.606 ug/L

RT: 10.142 min Scan# 1354

Delta R.T. 0.073 min

Lab File: VW030685.D




Acq: 21 Oct 2024 17:13


Tgt Ion: 75 Resp: 48

Ion Ratio Lower Upper

75 100

77 85.5 21.1 39.1#

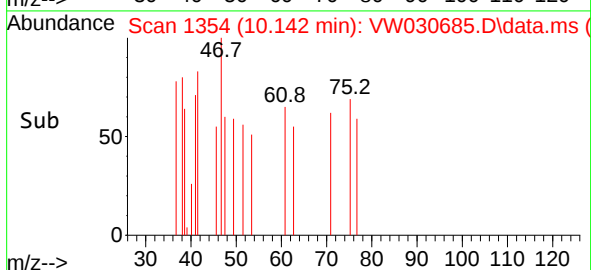



#40

4-Methyl-2-pentanone

Concen: 1.823 ug/L

RT: 10.221 min Scan# 1367

Delta R.T. 0.012 min

Lab File: VW030685.D





Acq: 21 Oct 2024 17:13

Instrument :

MSVOA_W

ClientSampleId :

Tgt Ion: 43	Resp: 46
Ion Ratio	Lower Upper
43	100
58	0.0 31.4 47.2#
100	0.0 13.1 19.7#

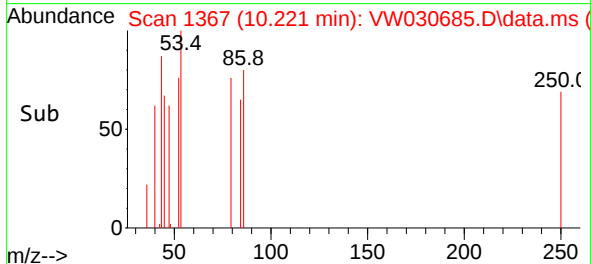

#42

Toluene

Concen: 1.110 ug/L




RT: 10.392 min Scan# 1395


Delta R.T. 0.006 min

Lab File: VW030685.D

Acq: 21 Oct 2024 17:13

Tgt Ion: 91	Resp: 249
Ion Ratio	Lower Upper
91	100
92	42.5 40.3 74.8

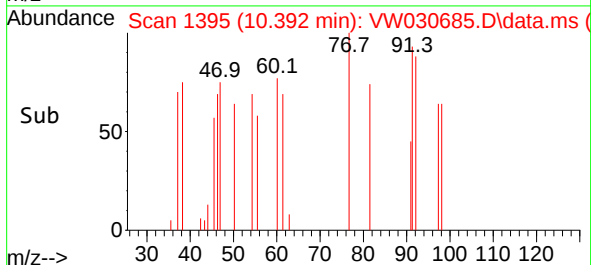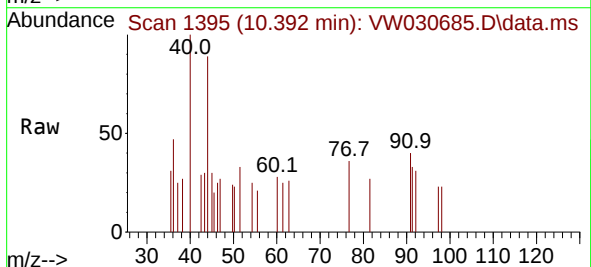



#44

trans-1,3-Dichloropropene

Concen: 0.976 ug/L

RT: 10.617 min Scan# 1432

Delta R.T. 0.012 min

Lab File: VW030685.D

Acq: 21 Oct 2024 17:13

Instrument :

MSVOA_W





ClientSampleId :

Tgt Ion: 75 Resp: 65

Ion Ratio Lower Upper

75 100

77 142.4 21.6 40.2#

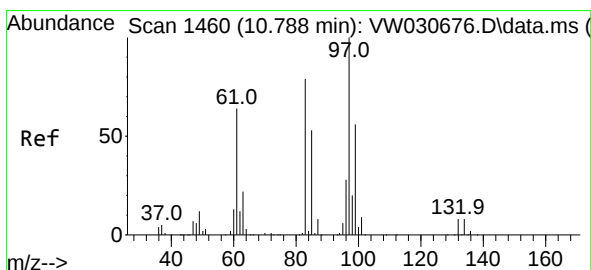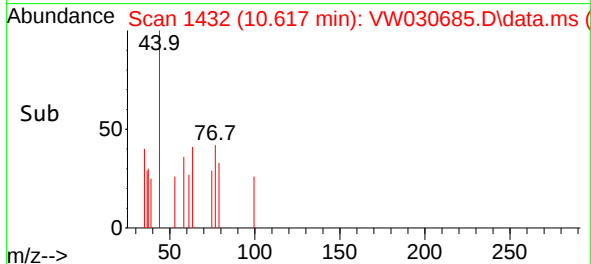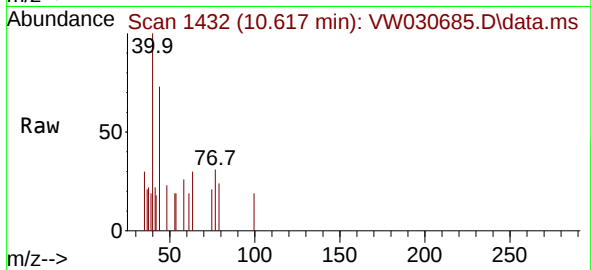

#45

1,1,2-Trichloroethane

Concen: 3.214 ug/L

RT: 10.660 min Scan# 1439

Delta R.T. -0.128 min

Lab File: VW030685.D

Acq: 21 Oct 2024 17:13

Tgt Ion: 97 Resp: 122




Ion Ratio Lower Upper


97 100

99 0.0 41.2 76.6#

83 0.0 59.6 110.6#

85 0.0 37.7 69.9#

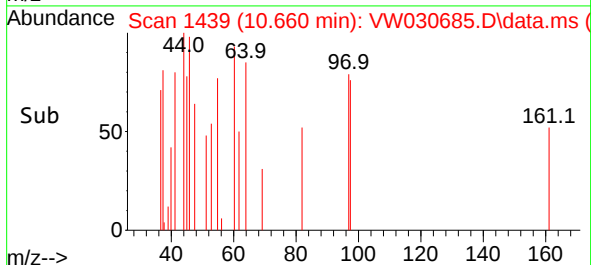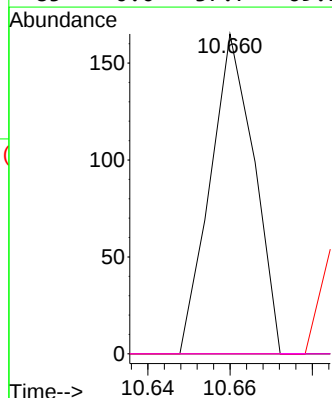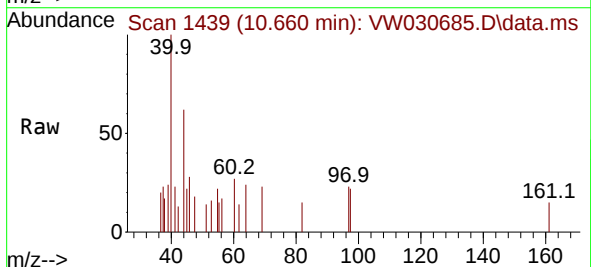



#49

Dibromochloromethane

Concen: 1.723 ug/L

RT: 11.032 min Scan# 11

Delta R.T. -0.091 min

Lab File: VW030685.D

Acq: 21 Oct 2024 17:13

Instrument :

MSVOA_W





ClientSampleId :

Tgt Ion:129 Resp: 73

Ion Ratio Lower Upper

129 100

127 0.0 56.5 104.9#

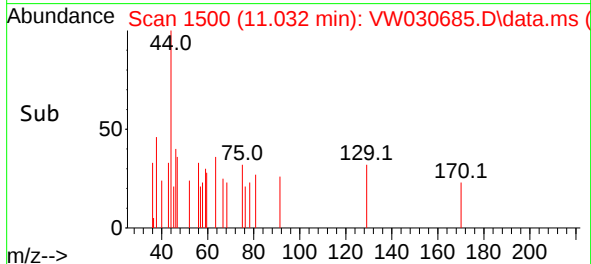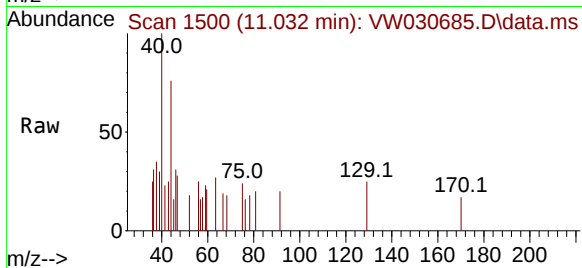

#53

m,p-Xylene

Concen: 0.511 ug/L

RT: 11.733 min Scan# 1615

Delta R.T. -0.104 min

Lab File: VW030685.D




Acq: 21 Oct 2024 17:13


Tgt Ion:106 Resp: 49

Ion Ratio Lower Upper

106 100

91 75.3 140.6 261.2#


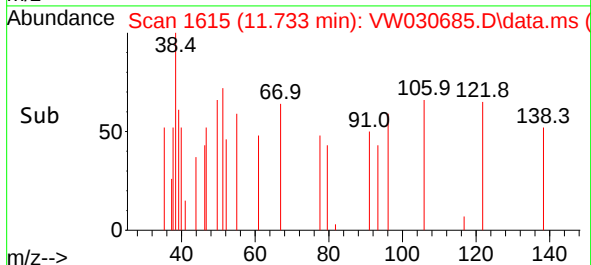

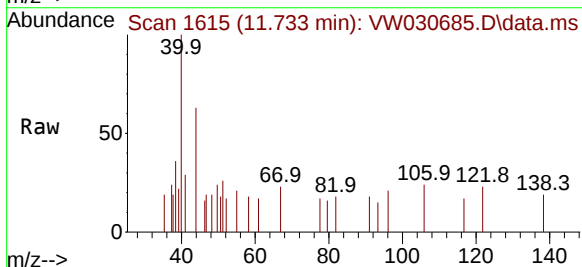




#54
o-Xylene
Concen: 0.485 ug/L
RT: 12.306 min Scan# 11
Delta R.T. 0.146 min
Lab File: VW030685.D
Acq: 21 Oct 2024 17:13




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion:106 Resp: 43
Ion Ratio Lower Upper
106 100
91 0.0 144.5 268.4#

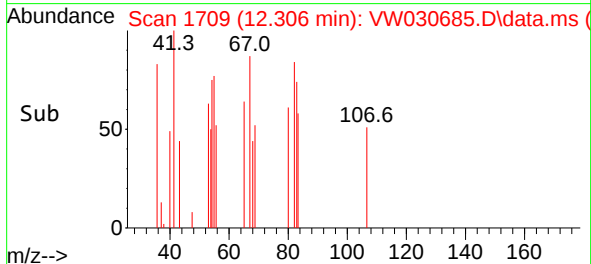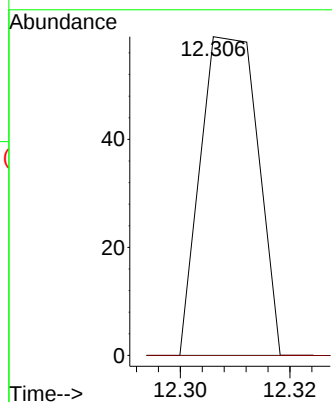

#55
Styrene
Concen: 0.376 ug/L
RT: 11.983 min Scan# 1656
Delta R.T. -0.195 min
Lab File: VW030685.D
Acq: 21 Oct 2024 17:13

Tgt Ion:104 Resp: 57
Ion Ratio Lower Upper
104 100
78 0.0 34.3 63.7#

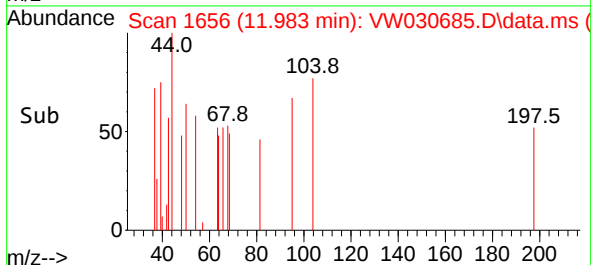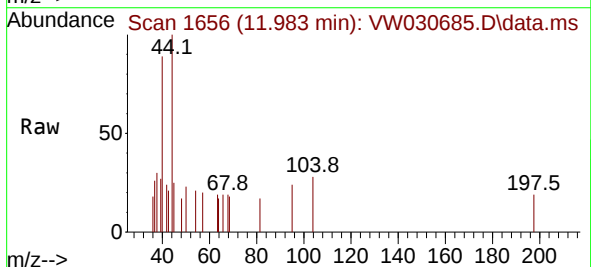



#57

1,1,2-Tetrachloroethane

Concen: 0.491 ug/L

RT: 12.751 min Scan# 1782

Delta R.T. 0.043 min

Lab File: VW030685.D




Acq: 21 Oct 2024 17:13

Instrument :

MSVOA_W

ClientSampleId :

Tgt Ion:	83	Resp:	21
Ion	Ratio	Lower	Upper
83	100		
85	0.0	42.6	79.2#
131	0.0	7.4	11.0#



#61

1,2,3-Trichloropropane

Concen: 2.635 ug/L




RT: 12.775 min Scan# 1786


Delta R.T. 0.012 min

Lab File: VW030685.D

Acq: 21 Oct 2024 17:13

Tgt Ion:	75	Resp:	54
Ion	Ratio	Lower	Upper
75	100		
77	77.8	25.7	38.5#
110	0.0	32.3	48.5#


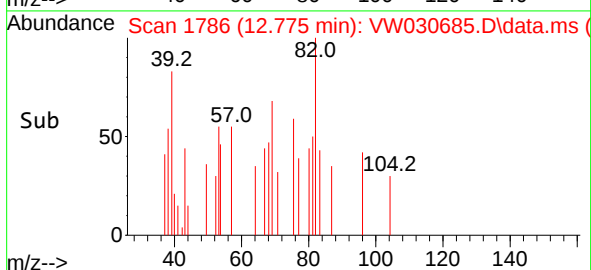






#63
1,2,4-Trimethylbenzene
Concen: 0.381 ug/L
RT: 13.227 min Scan# 11
Delta R.T. -0.018 min
Lab File: VW030685.D
Acq: 21 Oct 2024 17:13




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion:105 Resp: 48
Ion Ratio Lower Upper
105 100
120 0.0 35.8 53.6#

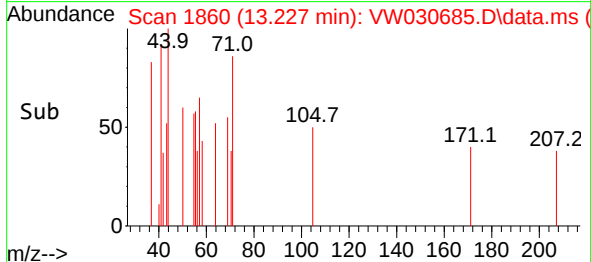

#64
1,3-Dichlorobenzene
Concen: 0.634 ug/L
RT: 13.574 min Scan# 1917
Delta R.T. 0.079 min
Lab File: VW030685.D
Acq: 21 Oct 2024 17:13


Tgt Ion:146 Resp: 45
Ion Ratio Lower Upper
146 100
111 0.0 31.2 58.0#
148 0.0 45.7 84.9#

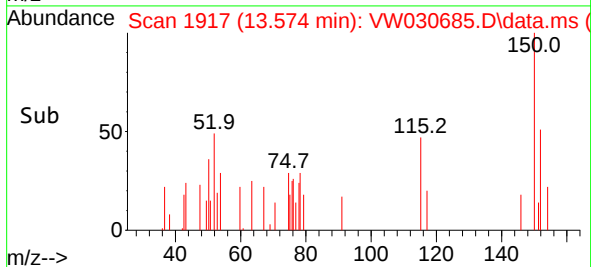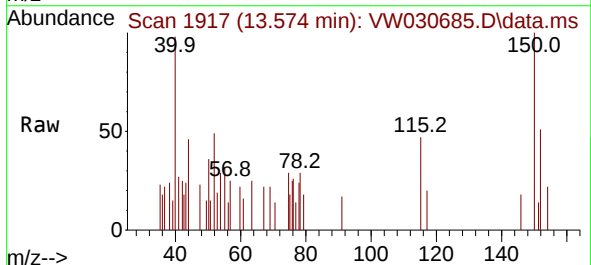






#65
1,4-Dichlorobenzene
Concen: 0.614 ug/L
RT: 13.574 min Scan# 1917
Delta R.T. 0.000 min
Lab File: VW030685.D
Acq: 21 Oct 2024 17:13


Instrument :
MSVOA_W
ClientSampleId :





Tgt Ion:146 Resp: 45
Ion Ratio Lower Upper
146 100
111 0.0 26.8 49.8#
148 0.0 41.0 76.2#

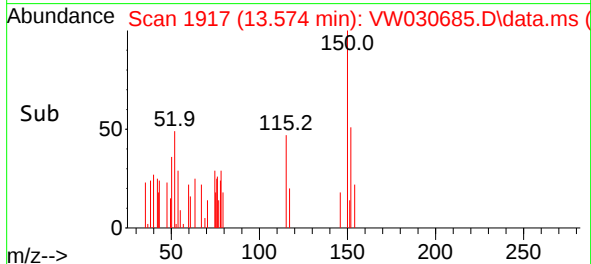


#67
1,2-Dichlorobenzene
Concen: 0.688 ug/L
RT: 14.111 min Scan# 2005
Delta R.T. 0.244 min
Lab File: VW030685.D
Acq: 21 Oct 2024 17:13

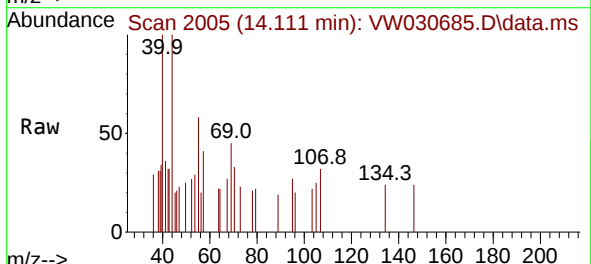


Tgt Ion:146 Resp: 43
Ion Ratio Lower Upper
146 100
111 0.0 34.6 52.0#
148 0.0 53.3 79.9#

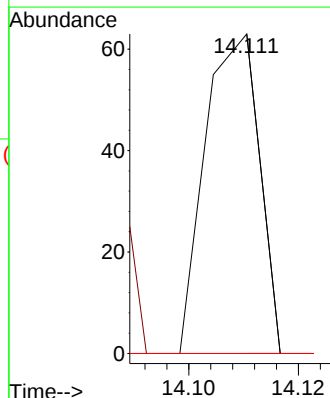



#71
Naphthalene
Concen: 0.783 ug/L
RT: 15.458 min Scan# 21
Delta R.T. 0.098 min
Lab File: VW030685.D
Acq: 21 Oct 2024 17:13

Instrument :
MSVOA_W
ClientSampleId :

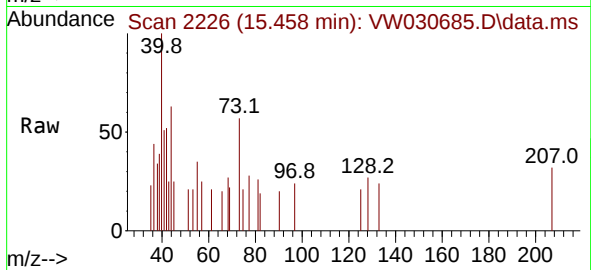

Tgt Ion:128 Resp: 51
Ion Ratio Lower Upper
128 100
127 0.0 10.9 16.3#
129 0.0 8.8 13.2#

