

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102124\
 Data File : VW030681.D
 Acq On : 21 Oct 2024 15:38
 Operator : SY/MD
 Sample : P4415-08
 Misc : 5.57g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4F60

Manual Integrations
 APPROVED

Reviewed By :Romaben Patel 10/22/2024
 Supervised By :Mahesh Dadoda 10/22/2024

Quant Time: Oct 22 01:35:18 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Oct 22 01:33:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	296201	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	231152	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	83576	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	50076	10.756	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	43.040%		
7) Chloroethane-d5	2.899	69	50917	14.448	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	57.800%		
11) 1,1-Dichloroethene-d2	4.021	65	20596	10.636	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	42.560%#		
21) 2-Butanone-d5	7.081	46	28841	34.422	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	68.840%		
24) Chloroform-d	7.648	84	146879	17.340	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	69.360%		
26) 1,2-Dichloroethane-d4	8.307	65	74585	16.933	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	67.720%#		
32) Benzene-d6	8.276	84	213673	15.927	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	63.720%		
36) 1,2-Dichloropropane-d6	9.276	67	78848	20.024	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	80.080%		
41) Toluene-d8	10.325	98	160513	13.106	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	52.440%		
43) trans-1,3-Dichloroprop...	10.581	79	26205	15.893	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	63.560%		
47) 2-Hexanone-d5	10.922	63	20142	39.714	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	79.420%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	58030	20.067	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	80.280%		
66) 1,2-Dichlorobenzene-d4	13.848	152	50269	17.776	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	71.120%#		
Target Compounds					Qvalue	
13) Acetone	4.124	43	18057	14.720	ug/L	99
22) 2-Butanone	7.179	43	7026m	5.314	ug/L	
42) Toluene	10.386	91	36223	2.257	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102124\
Data File : VW030681.D
Acq On : 21 Oct 2024 15:38
Operator : SY/MD
Sample : P4415-08
Misc : 5.57g/10mL/MSVOA_W/SOIL/A
ALS Vial : 8 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
A4F60

Manual Integrations
APPROVED

Reviewed By :Romaben Patel 10/22/2024
Supervised By :Mahesh Dadoda 10/22/2024


Quant Time: Oct 22 01:35:18 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Oct 22 01:33:40 2024
Response via : Initial Calibration

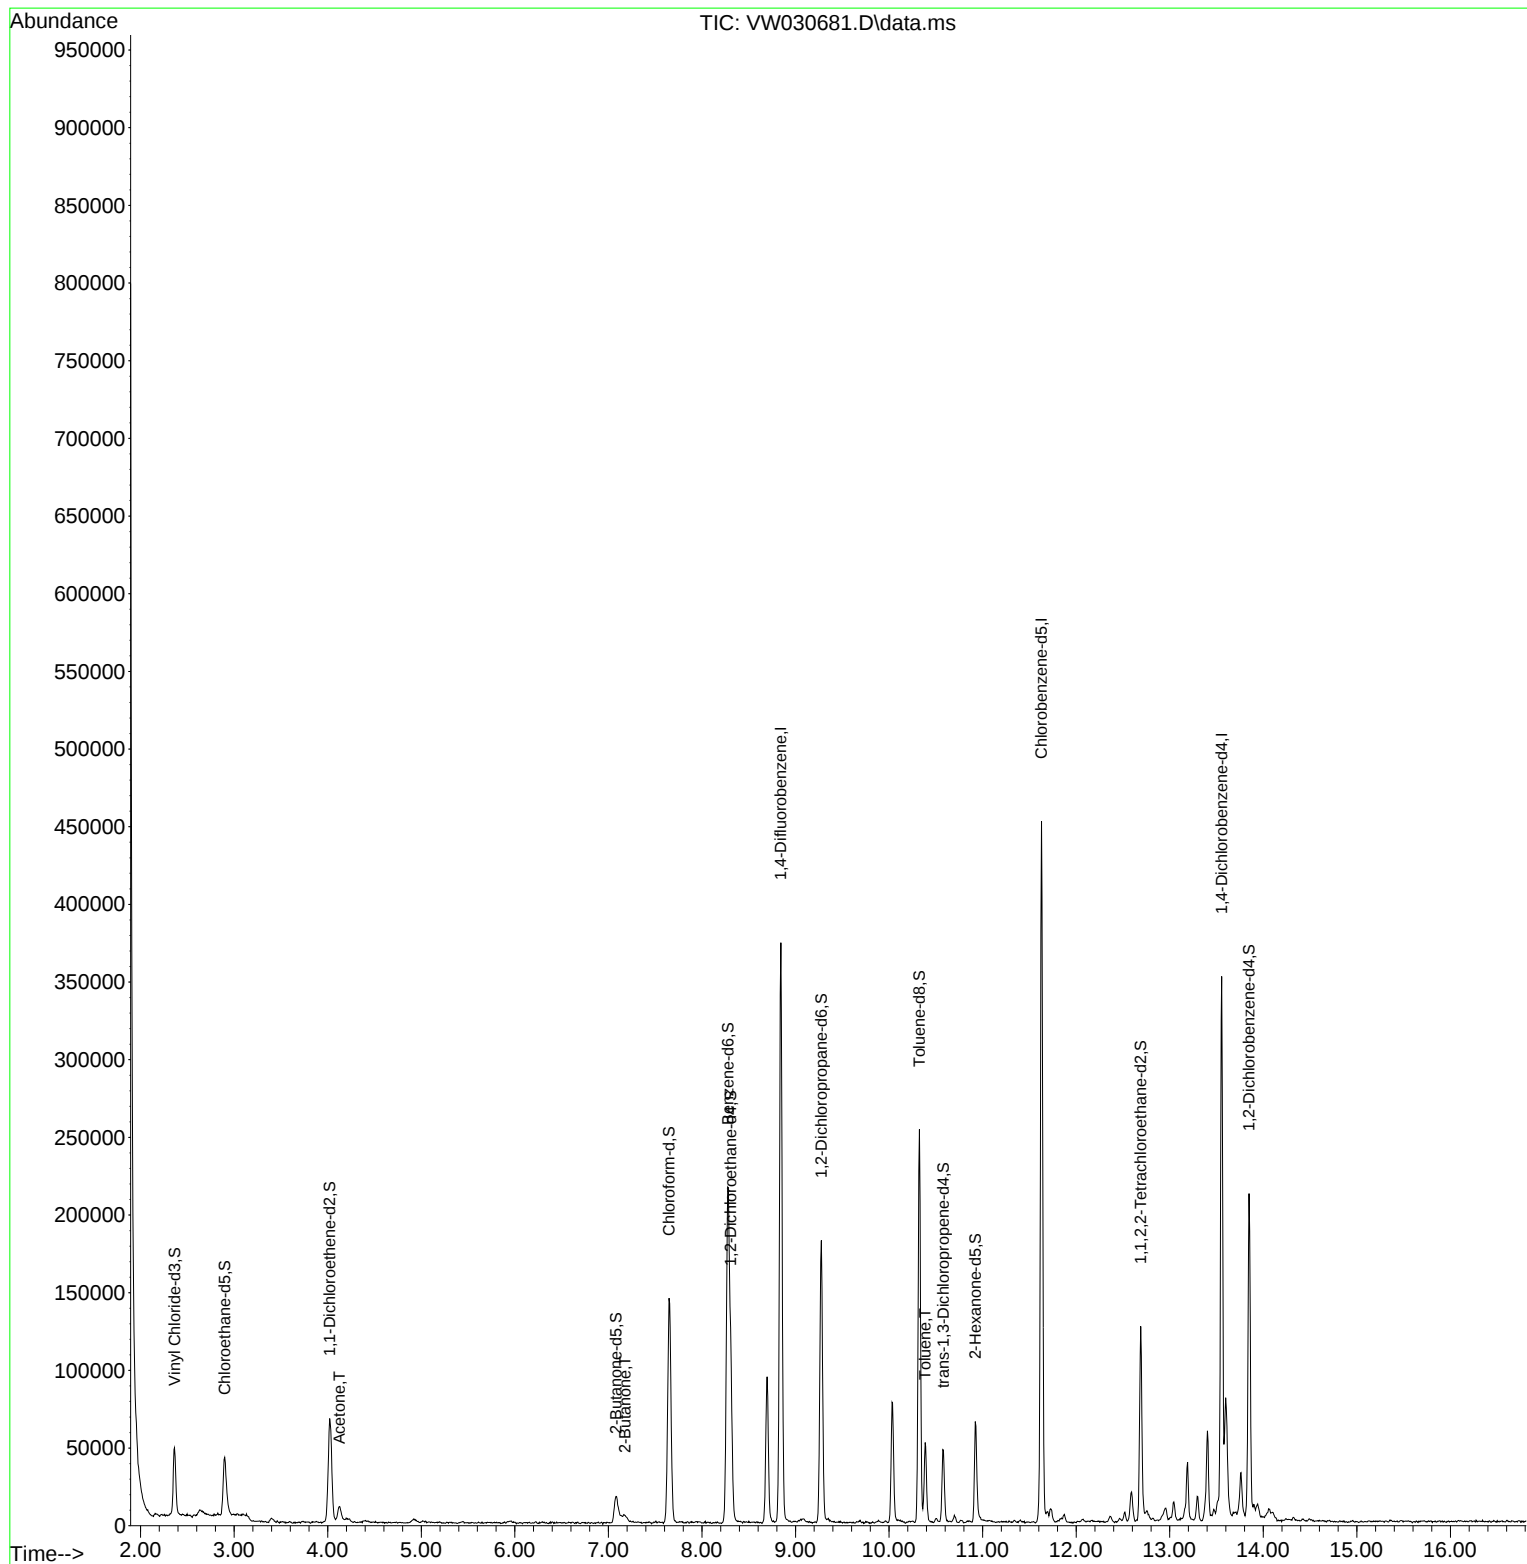

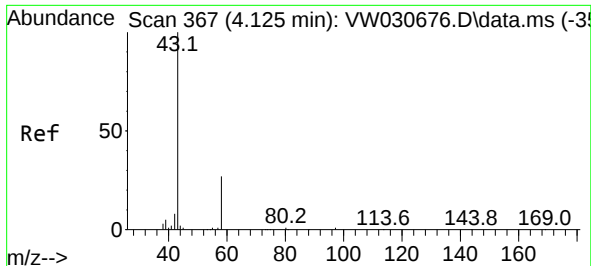

#13
Acetone
Concen: 14.720 ug/L
RT: 4.124 min Scan# 30
Delta R.T. -0.000 min
Lab File: VW030681.D
Acq: 21 Oct 2024 15:38




Instrument :
MSVOA_W
ClientSampleId :
A4F60

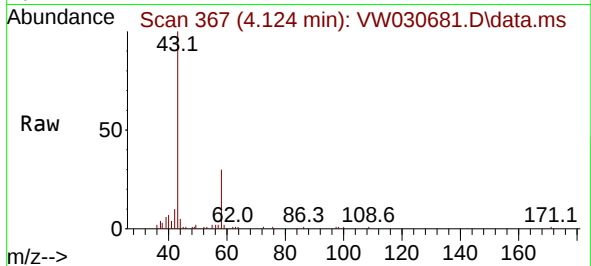

Tgt Ion: 43 Resp: 1805
Ion Ratio Lower Upper
43 100
58 29.6 0.0 57.6




Manual Integrations
APPROVED


Reviewed By :Romaben Patel 10/22/2024
Supervised By :Mahesh Dadoda 10/22/2024

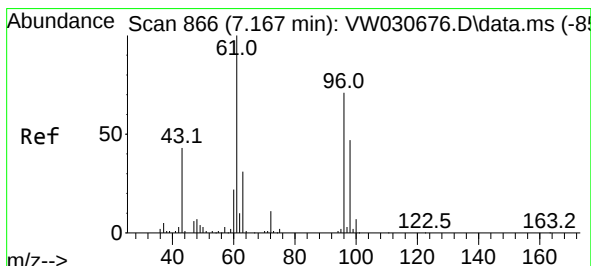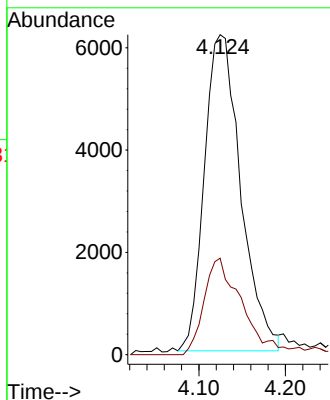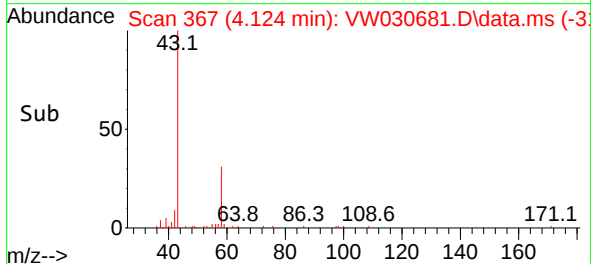

#22
2-Butanone
Concen: 5.314 ug/L m
RT: 7.179 min Scan# 868
Delta R.T. 0.012 min
Lab File: VW030681.D
Acq: 21 Oct 2024 15:38

Tgt Ion: 43 Resp: 7026
Ion Ratio Lower Upper
43 100
72 0.0 14.4 43.0#

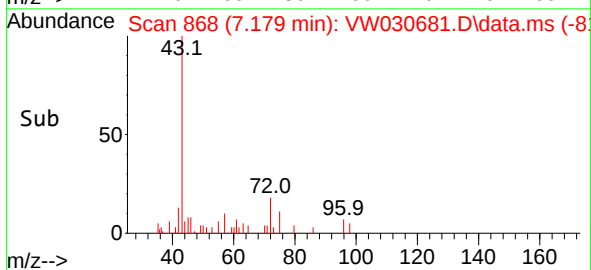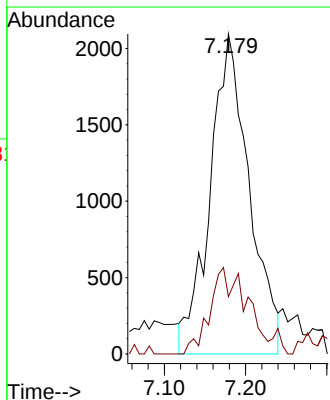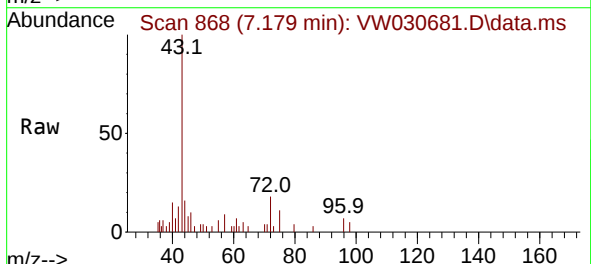

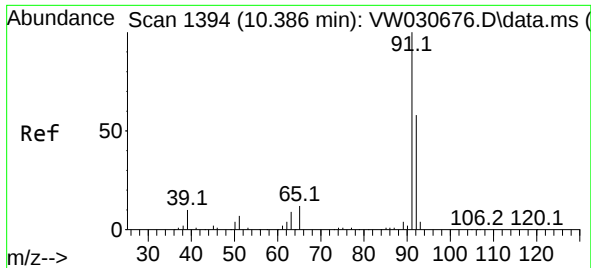

#42
Toluene
Concen: 2.257 ug/L
RT: 10.386 min Scan# 11
Delta R.T. -0.000 min
Lab File: VW030681.D
Acq: 21 Oct 2024 15:38

Instrument :
MSVOA_W
ClientSampleId :
A4F60

Tgt Ion: 91 Resp: 3622
Ion Ratio Lower Upper
91 100
92 56.0 40.3 74.8

Manual Integrations
APPROVED

Reviewed By :Romaben Patel 10/22/2024
Supervised By :Mahesh Dadoda 10/22/2024

