

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102124\
 Data File : VW030685.D
 Acq On : 21 Oct 2024 17:13
 Operator : SY/MD
 Sample : P4415-13
 Misc : 3.48g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4F81

Quant Time: Oct 22 01:36:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Oct 22 01:33:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.849	114	3138	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.629	117	3232	25.000	ug/L	# 0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	1053	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	723	14.658	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	58.640%
7) Chloroethane-d5	2.905	69	889	23.810	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.240%
11) 1,1-Dichloroethene-d2	0.000	65	0d	0.000	ug/L	
Spiked Amount	25.000	Range	45 - 110	Recovery	=	0.000%#
21) 2-Butanone-d5	0.000	46	0d	0.000	ug/L	
Spiked Amount	50.000	Range	20 - 135	Recovery	=	0.000%#
24) Chloroform-d	7.654	84	2931	32.661	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	130.640%
26) 1,2-Dichloroethane-d4	8.307	65	2215	47.466	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	189.880%#
32) Benzene-d6	8.276	84	3517	18.749	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	75.000%
36) 1,2-Dichloropropane-d6	9.276	67	1822	33.092	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	132.360%#
41) Toluene-d8	10.331	98	2014	11.761	ug/L	0.01
Spiked Amount	25.000	Range	30 - 130	Recovery	=	47.040%
43) trans-1,3-Dichloroprop...	10.587	79	441	19.128	ug/L	0.01
Spiked Amount	25.000	Range	30 - 135	Recovery	=	76.520%
47) 2-Hexanone-d5	0.000	63	0d	0.000	ug/L	
Spiked Amount	50.000	Range	20 - 135	Recovery	=	0.000%#
56) 1,1,2,2-Tetrachloroeth...	12.690	84	2016	49.859	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	199.440%#
66) 1,2-Dichlorobenzene-d4	13.855	152	991	27.814	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	111.240%
Target Compounds						
13) Acetone	4.137	43	1405	108.114	ug/L	Qvalue 80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102124\
Data File : VW030685.D
Acq On : 21 Oct 2024 17:13
Operator : SY/MD
Sample : P4415-13
Misc : 3.48g/10mL/MSVOA_W/SOIL/A
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4F81


Quant Time: Oct 22 01:36:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Oct 22 01:33:40 2024
Response via : Initial Calibration

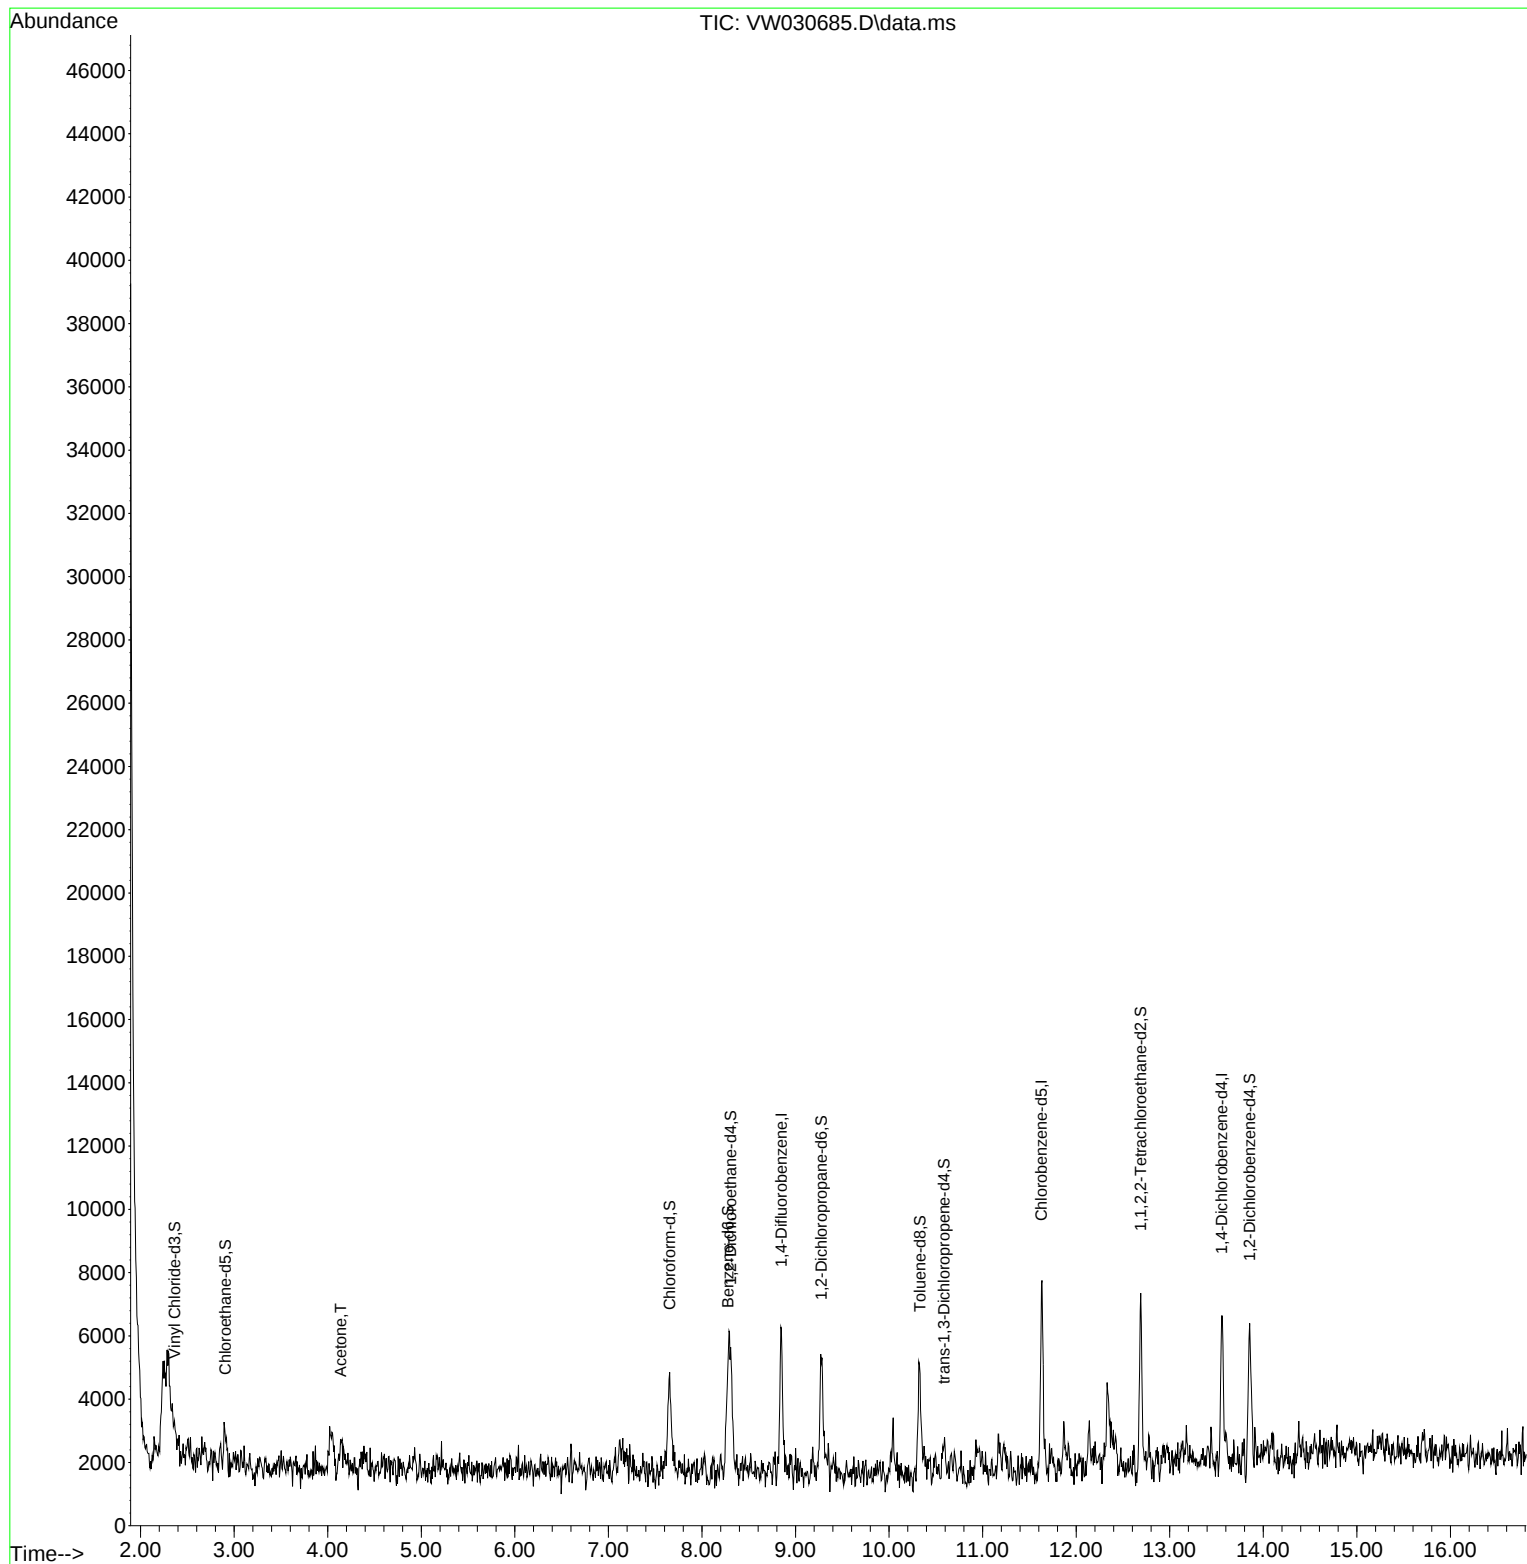

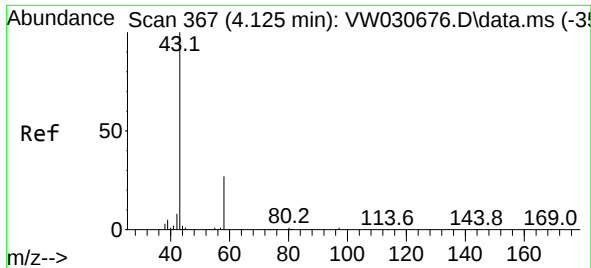

#13
 Acetone
 Concen: 108.114 ug/L
 RT: 4.137 min Scan# 30
 Delta R.T. 0.012 min
 Lab File: VW030685.D
 Acq: 21 Oct 2024 17:13

Instrument :
 MSVOA_W
 ClientSampleId :
 A4F81

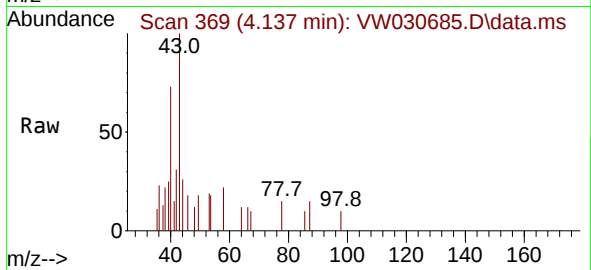

Tgt Ion: 43 Resp: 1405
 Ion Ratio Lower Upper
 43 100
 58 18.4 0.0 57.6

