
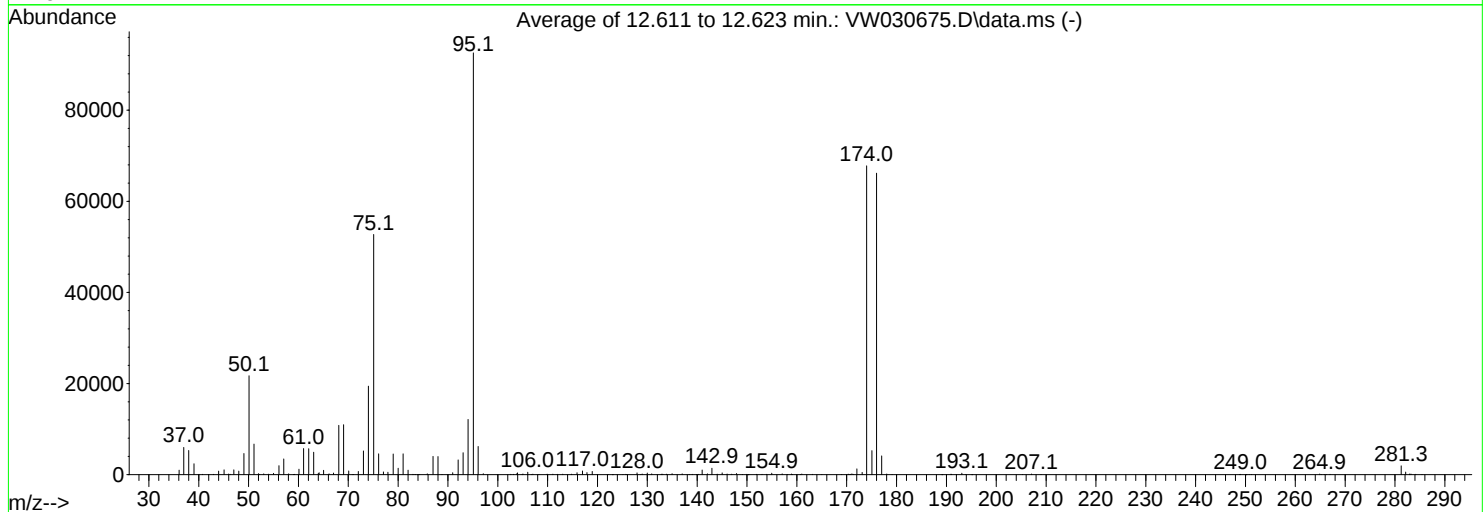


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102124\
Data File : VW030675.D
Acq On : 21 Oct 2024 08:52
Operator : SY/MD
Sample : BFB580
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB580

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Title : SFAM01.0
Last Update : Tue Oct 22 01:33:40 2024

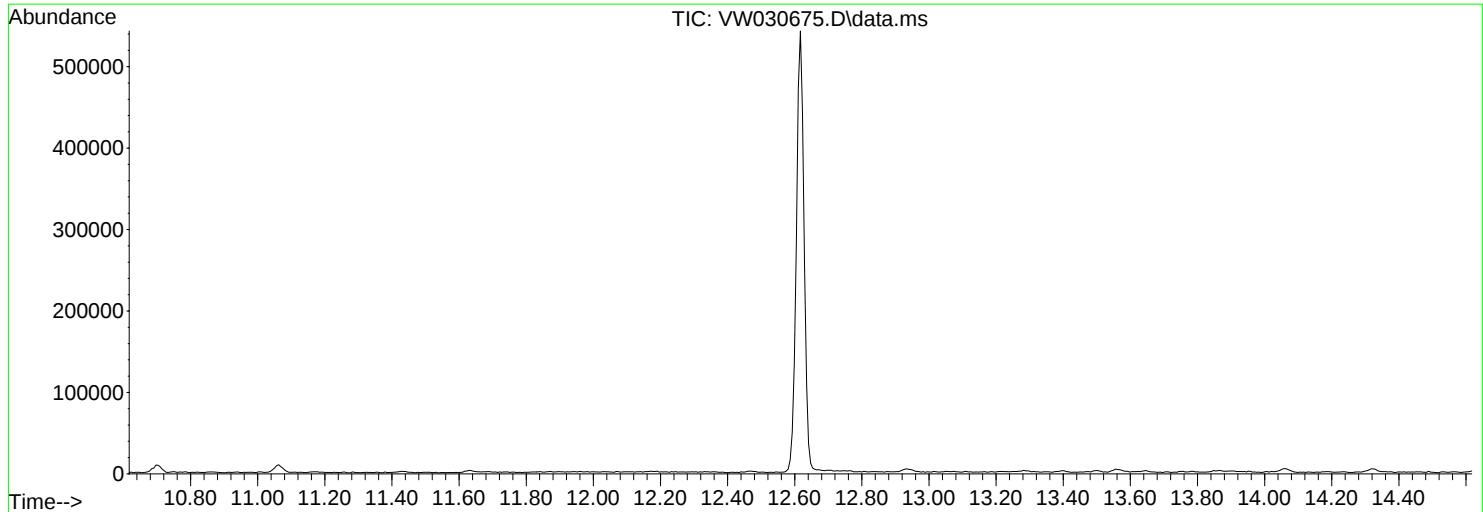

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.4	21695	PASS
75	95	30	80	56.9	52715	PASS
95	95	100	100	100.0	92600	PASS
96	95	5	9	6.7	6178	PASS
173	174	0.00	2	0.7	505	PASS
174	95	50	120	73.2	67787	PASS
175	174	5	9	7.8	5266	PASS
176	174	95	101	97.6	66179	PASS
177	176	5	9	6.2	4104	PASS

m/z	Abundance
35.10	105.0
36.10	266.0
36.90	105.0
38.00	164.0
38.70	70.0
39.30	120.0
40.00	295.0
41.20	120.0
42.40	54.0
43.10	77.0
44.00	228.0
45.30	59.0
46.00	56.0
46.70	58.0
50.20	60.0
55.10	101.0
56.40	60.0
57.70	56.0
60.80	50.0
61.50	58.0
68.40	64.0

Instrument :
MSVOA_W
ClientSampleId :
BFB580

m/z	Abundance
36.00	1326.0
37.00	6259.0
38.00	6014.0
39.00	2464.0
40.10	438.0
40.80	75.0
41.20	68.0
42.00	96.0
43.10	172.0
44.10	942.0
45.10	1243.0
46.10	308.0
47.10	1046.0
48.10	771.0
49.00	4447.0
50.10	21704.0
51.10	6699.0
52.00	365.0
53.10	220.0
54.00	120.0
55.00	485.0
56.10	1941.0
57.10	3517.0
58.10	191.0
59.00	128.0
60.10	1115.0
61.10	5929.0
62.10	5882.0
63.00	5265.0
64.00	845.0
65.10	1097.0
66.20	177.0
67.10	350.0
68.10	10724.0
69.00	10775.0
70.10	783.0
70.80	91.0
72.00	663.0
73.00	5085.0
74.00	18664.0
75.10	52328.0
76.10	4670.0
77.00	542.0
78.00	553.0
79.00	4537.0
80.00	1393.0
81.00	4646.0
82.00	1236.0
83.00	127.0
83.50	53.0
85.80	171.0
87.00	3959.0
88.00	3775.0
88.80	105.0
90.90	409.0
92.00	2948.0
93.10	5169.0
94.10	10457.0
95.10	88344.0
96.00	6466.0
97.10	249.0
103.10	136.0
103.80	498.0
104.90	250.0
106.00	512.0
107.10	168.0
109.80	125.0
111.10	112.0
113.00	82.0
114.80	86.0
115.90	401.0
117.00	846.0
117.80	446.0
118.90	687.0
125.70	169.0
127.90	330.0
128.70	88.0
129.00	121.0
130.00	339.0
130.90	144.0
133.10	313.0
133.90	164.0
134.90	231.0
137.00	163.0
138.40	67.0
139.00	55.0
139.90	106.0
141.00	959.0
142.10	190.0
143.00	1653.0
144.00	99.0
145.00	450.0

Instrument :
MSVOA_W
ClientSampleId :
BFB580

146.10	102.0
146.90	170.0
147.90	201.0
149.10	130.0
149.90	121.0
154.00	104.0
155.00	188.0
157.00	198.0
158.10	59.0
158.90	158.0
161.00	136.0
163.10	106.0
165.10	61.0
170.30	123.0
170.80	180.0
171.30	245.0
172.10	1231.0
174.00	62760.0
175.00	4784.0
176.00	61264.0
177.00	3565.0
178.10	164.0
179.10	115.0
189.10	51.0
190.90	279.0
192.00	64.0
193.10	502.0
193.90	81.0
195.10	50.0
205.30	76.0
207.10	280.0
209.00	63.0
248.80	130.0
250.10	55.0
251.20	71.0
264.90	342.0
266.90	125.0
281.20	3302.0
282.20	858.0
283.20	460.0
284.20	123.0
285.40	73.0

Instrument :
MSVOA_W
ClientSampleId :
BFB580

m/z	Abundance
36.00	1220.0
37.10	6773.0
38.10	5959.0
39.10	2543.0
40.10	395.0
40.70	127.0
42.20	71.0
42.90	211.0
44.10	1211.0
45.10	1256.0
46.00	287.0
47.00	1156.0
47.90	792.0
49.10	5579.0
50.10	24968.0
51.10	7301.0
52.00	274.0
53.10	180.0
54.00	82.0
55.00	347.0
56.10	2255.0
57.00	3617.0
58.00	216.0
59.20	131.0
60.10	1693.0
61.00	6491.0
62.10	6195.0
63.10	5524.0
64.20	621.0
65.00	801.0
66.20	176.0
67.10	458.0
68.10	12048.0
69.10	12651.0
70.10	1057.0
71.00	71.0
72.10	906.0
73.10	5774.0
74.10	21904.0
75.10	60144.0
76.10	5038.0
77.10	616.0
77.90	563.0
79.00	5052.0
80.00	1614.0
81.00	5179.0
82.00	939.0
82.90	92.0
83.50	76.0
84.30	59.0
85.80	184.0
87.00	4779.0
88.00	4553.0
91.00	446.0
92.10	3607.0
93.00	5049.0
94.10	14156.0
95.10	103808.0
96.10	6655.0
97.10	194.0
102.60	106.0
104.00	665.0
105.10	208.0
106.00	584.0
107.00	144.0
108.20	51.0
109.90	133.0
111.10	143.0
112.00	106.0
113.10	130.0
114.90	123.0
115.90	460.0
117.00	954.0
117.90	461.0
119.00	795.0
122.10	59.0
125.10	66.0
125.80	54.0
127.90	479.0
128.90	214.0
130.00	470.0
130.90	241.0
132.80	163.0
133.80	96.0
134.90	183.0
137.00	190.0
139.00	94.0
140.20	195.0
141.00	1009.0
142.00	205.0
142.90	1485.0
144.00	96.0

Instrument :
MSVOA_W
ClientSampleId :
BFB580

145.10	444.0
145.90	148.0
146.90	56.0
147.90	299.0
150.00	135.0
151.90	170.0
153.00	96.0
153.90	122.0
155.00	404.0
157.00	187.0
158.90	149.0
160.90	145.0
163.10	93.0
164.90	86.0
169.00	62.0
170.30	162.0
171.00	245.0
172.10	1142.0
174.00	77920.0
175.10	5777.0
176.00	70824.0
177.00	4981.0
178.10	94.0
191.10	170.0
193.10	266.0
193.90	65.0
207.10	119.0
249.00	191.0
250.80	67.0
265.20	165.0
265.80	61.0
267.00	119.0
281.30	1502.0
282.00	478.0
282.90	269.0
284.10	91.0

Instrument :
MSVOA_W
ClientSampleId :
BFB580

m/z	Abundance
36.10	1262.0
37.10	5228.0
38.10	4382.0
39.10	2149.0
40.00	276.0
41.00	115.0
42.80	87.0
44.00	897.0
45.00	829.0
46.30	229.0
47.00	989.0
48.10	727.0
49.10	3923.0
50.10	18592.0
51.10	6169.0
52.20	183.0
53.00	183.0
54.10	88.0
55.00	353.0
56.10	1764.0
57.10	3237.0
58.00	146.0
59.20	96.0
60.10	800.0
61.00	4746.0
62.00	5050.0
63.10	3939.0
64.10	610.0
65.10	948.0
66.10	140.0
66.90	201.0
68.10	9686.0
69.10	9478.0
70.10	578.0
71.10	74.0
71.90	521.0
73.10	4795.0
74.10	17688.0
75.10	45672.0
76.10	3995.0
77.10	595.0
77.90	445.0
79.00	4012.0
80.00	1184.0
81.00	3846.0
82.00	784.0
83.20	141.0
83.90	57.0
85.90	196.0
87.00	3283.0
88.00	3550.0
91.00	385.0
92.10	3096.0
93.10	4274.0
94.00	11737.0
95.10	85648.0
96.00	5412.0
97.10	159.0
102.60	77.0
103.20	77.0
103.90	532.0
105.00	219.0
106.00	537.0
106.80	146.0
108.30	52.0
110.00	98.0
111.00	120.0
111.90	95.0
113.00	108.0
114.70	102.0
115.90	373.0
117.00	634.0
118.00	490.0
119.00	626.0
122.10	76.0
123.00	51.0
125.10	56.0
125.90	157.0
128.00	337.0
128.90	125.0
130.00	232.0
131.00	119.0
132.80	158.0
133.80	71.0
135.00	189.0
137.00	171.0
139.00	61.0
141.00	1095.0
142.10	178.0
143.00	1115.0
144.00	138.0
144.90	249.0

Instrument :
MSVOA_W
ClientSampleId :
BFB580

146.00	194.0
147.00	94.0
147.90	300.0
150.20	57.0
153.00	123.0
154.90	310.0
157.10	200.0
158.80	101.0
159.10	109.0
160.70	138.0
161.10	107.0
170.50	163.0
171.10	252.0
172.00	1426.0
173.10	1515.0
174.00	62680.0
175.00	5237.0
176.00	66448.0
177.00	3767.0
178.00	179.0
191.00	68.0
193.10	141.0
207.20	51.0
249.00	57.0
250.70	55.0
265.00	109.0
266.20	96.0
281.20	963.0
282.10	311.0
282.90	124.0

Instrument :
MSVOA_W
ClientSampleId :
BFB580