

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102422\
 Data File : VW024964.D
 Acq On : 24 Oct 2022 14:17
 Operator : SY/VA
 Sample : VW1024SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK431

Quant Time: Oct 27 02:13:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 27 02:12:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	418010	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	385761	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	188330	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	93655	18.991	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	75.960%		
7) Chloroethane-d5	2.885	69	58432	20.237	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	80.960%		
11) 1,1-Dichloroethene-d2	4.019	63	154629	14.421	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	57.680%		
21) 2-Butanone-d5	7.079	46	77569	49.642	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	99.280%		
24) Chloroform-d	7.652	84	252104	21.383	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	85.520%		
26) 1,2-Dichloroethane-d4	8.305	65	137180	22.232	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	88.920%		
32) Benzene-d6	8.274	84	525488	21.723	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	86.880%		
36) 1,2-Dichloropropane-d6	9.274	67	165885	22.358	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	89.440%		
41) Toluene-d8	10.323	98	463921	21.367	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	85.480%		
43) trans-1,3-Dichloroprop...	10.579	79	62478	22.203	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	88.800%		
47) 2-Hexanone-d5	10.920	63	59666	47.966	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	95.940%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	132805	22.952	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	91.800%		
66) 1,2-Dichlorobenzene-d4	13.846	152	150021	21.798	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	87.200%		
Target Compounds						Qvalue
16) Methylene chloride	4.921	84	28071	3.803	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102422\
Data File : VW024964.D
Acq On : 24 Oct 2022 14:17
Operator : SY/VA
Sample : VW1024SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK431


Quant Time: Oct 27 02:13:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 27 02:12:22 2022
Response via : Initial Calibration

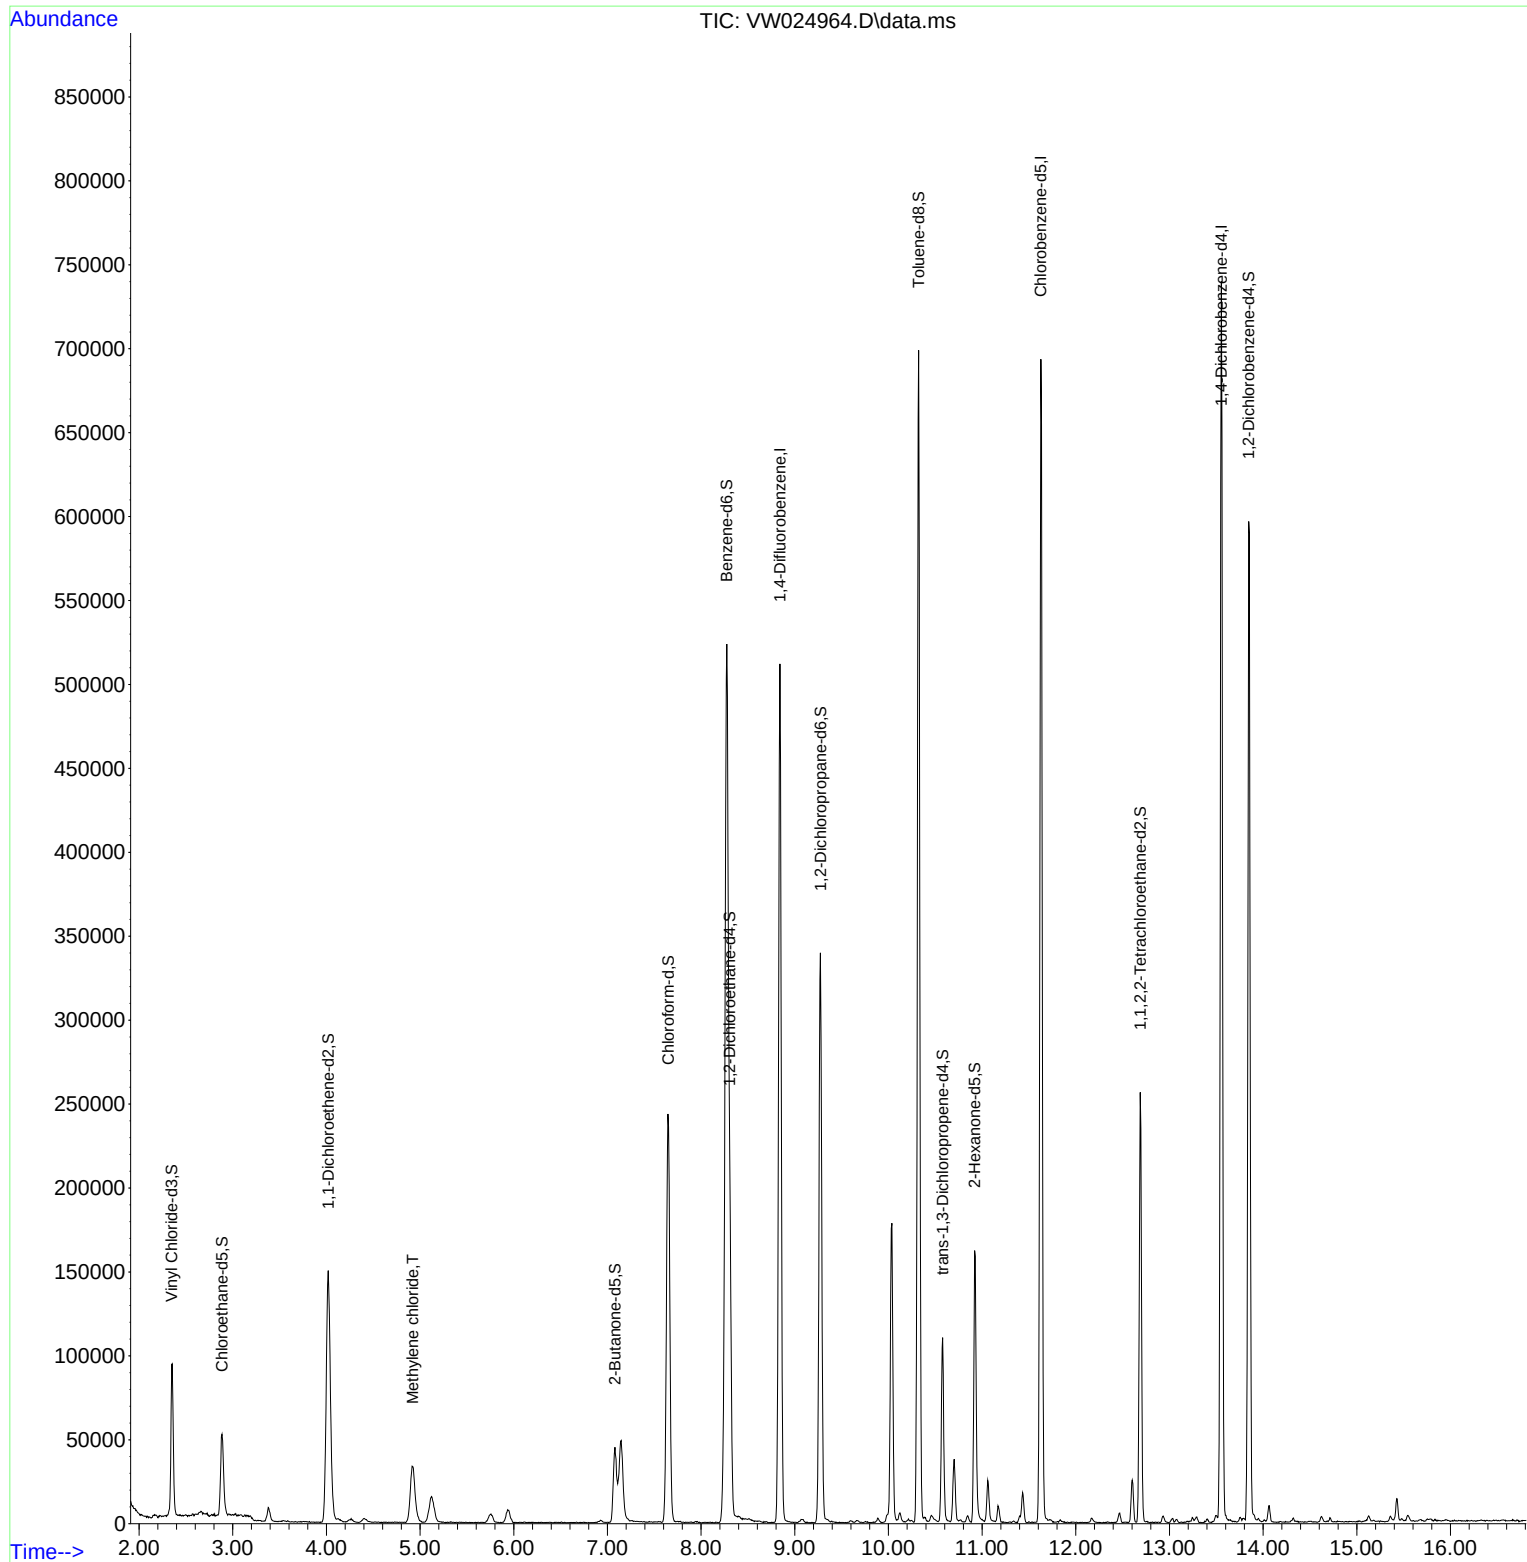

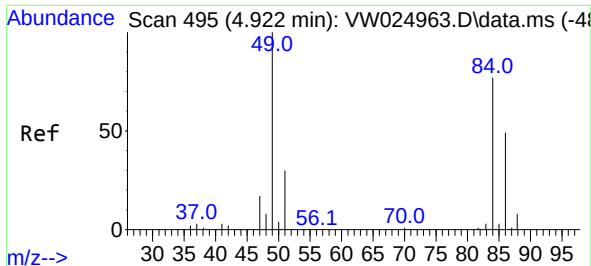

#16
Methylene chloride
Concen: 3.803 ug/L
RT: 4.921 min Scan# 49
Delta R.T. -0.000 min
Lab File: VW024964.D
Acq: 24 Oct 2022 14:17

Instrument :
MSVOA_W
ClientSampleId :
VBLK431

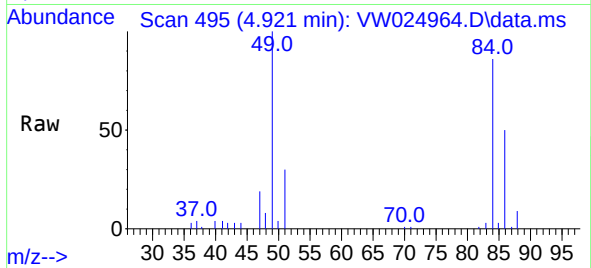

Tgt Ion: 84 Resp: 28071

Ion	Ratio	Lower	Upper
84	100		
86	58.1	45.5	84.5
49	116.8	90.9	168.9

