

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102423\
 Data File : VW027426.D
 Acq On : 24 Oct 2023 18:57
 Operator : SY/MD
 Sample : VIBLK549
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK549

Quant Time: Oct 25 01:34:21 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Oct 25 01:28:28 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	386190	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	355162	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	179247	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	107783	18.287	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	73.160%
7) Chloroethane-d5	2.899	69	88576	20.930	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.720%
11) 1,1-Dichloroethene-d2	4.021	65	57737	19.550	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	78.200%
21) 2-Butanone-d5	7.075	46	100131	51.114	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	102.220%
24) Chloroform-d	7.654	84	256968	22.325	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.280%
26) 1,2-Dichloroethane-d4	8.307	65	143311	23.178	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.720%
32) Benzene-d6	8.276	84	521894	21.719	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	86.880%
36) 1,2-Dichloropropane-d6	9.270	67	167933	22.881	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.520%
41) Toluene-d8	10.325	98	449743	20.640	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	82.560%
43) trans-1,3-Dichloroprop...	10.581	79	62126	18.565	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	74.280%
47) 2-Hexanone-d5	10.922	63	71965	47.392	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.780%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	136911	25.003	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.000%
66) 1,2-Dichlorobenzene-d4	13.848	152	146652	22.577	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.320%
Target Compounds						Qvalue
16) Methylene chloride	4.917	84	26569	3.758	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102423\
Data File : VW027426.D
Acq On : 24 Oct 2023 18:57
Operator : SY/MD
Sample : VIBLK549
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK549

Quant Time: Oct 25 01:34:21 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101123SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 25 01:28:28 2023
Response via : Initial Calibration

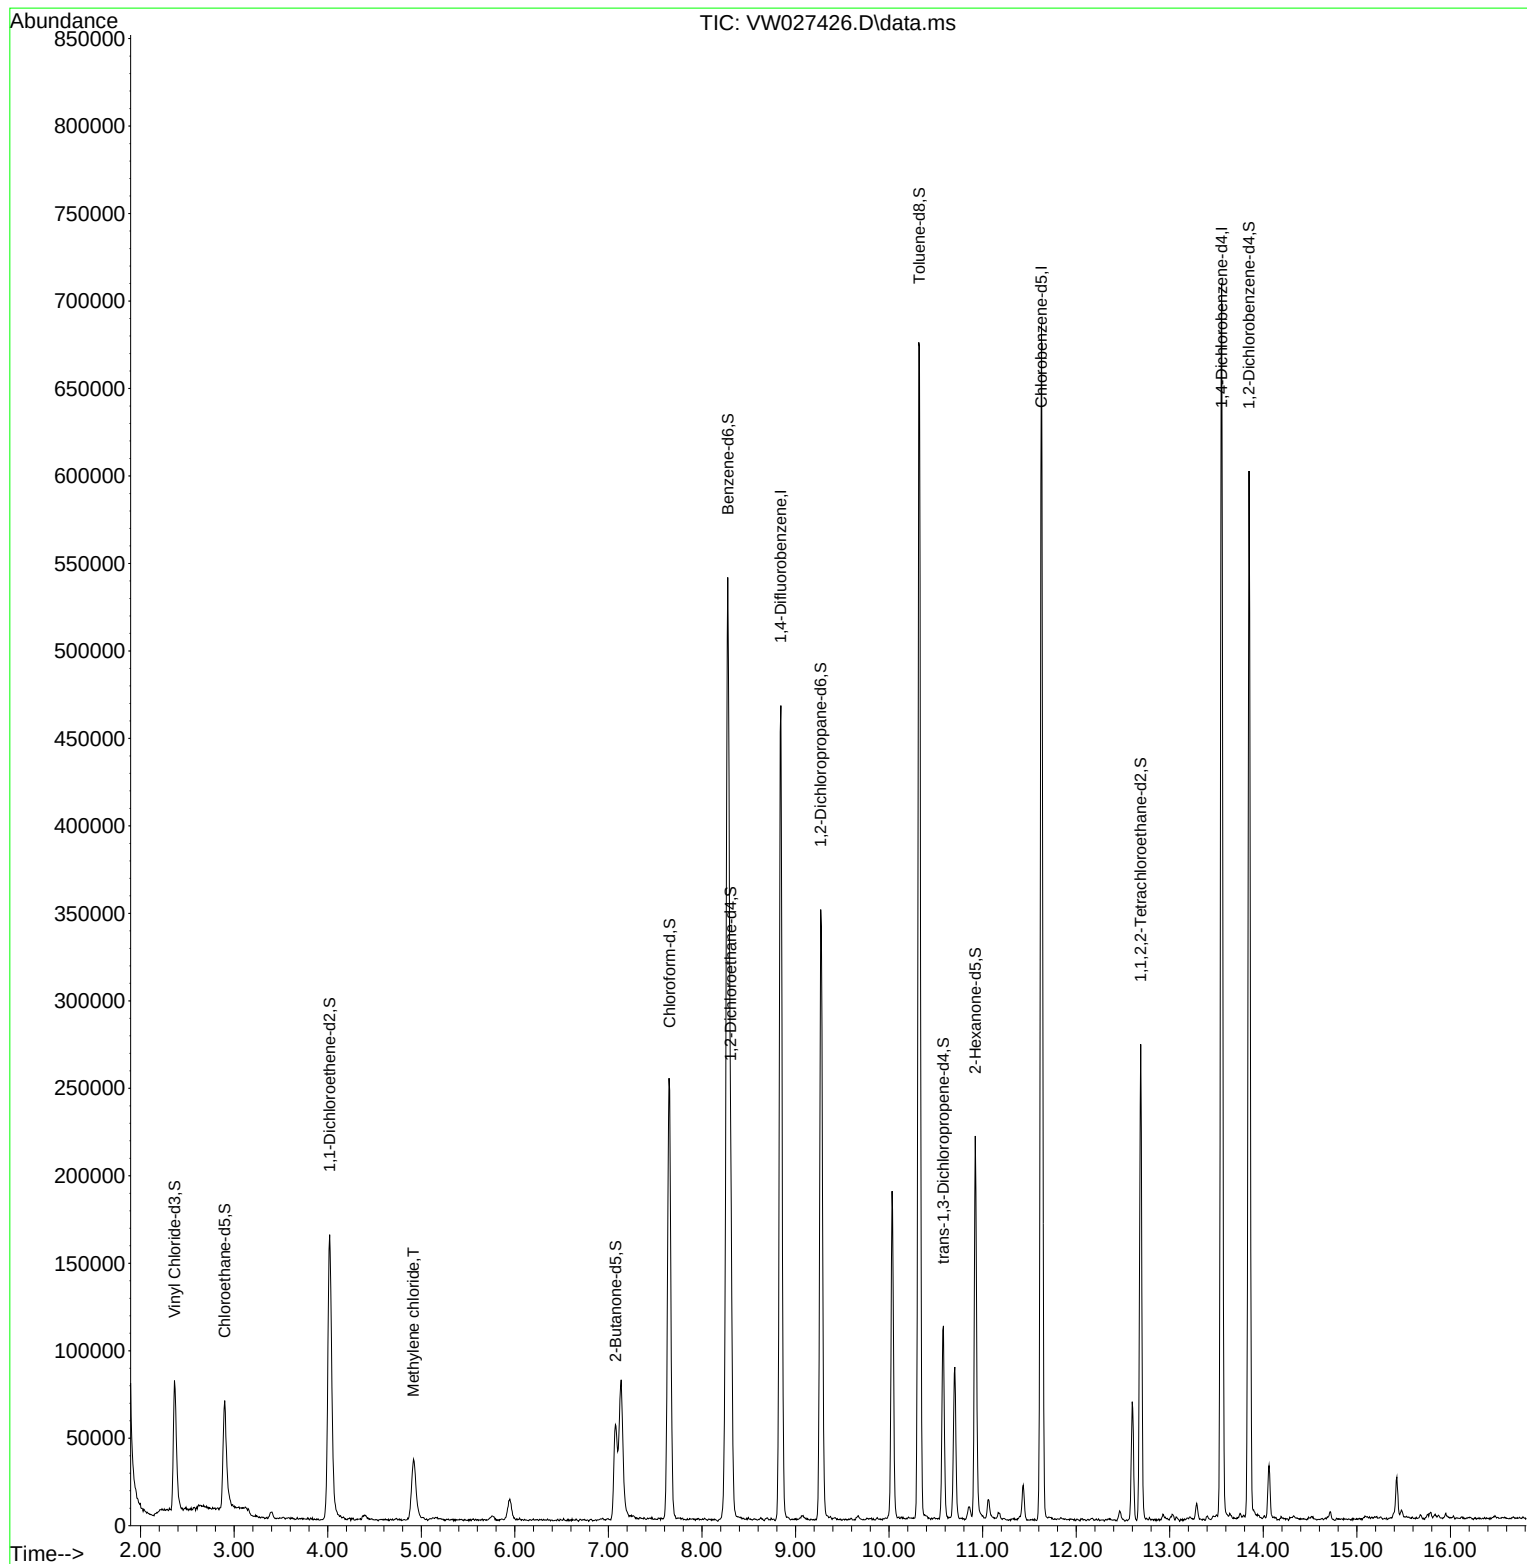

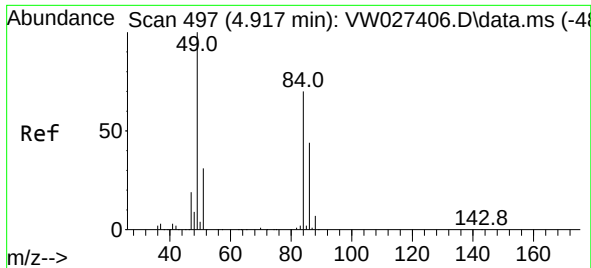

#16
Methylene chloride
Concen: 3.758 ug/L
RT: 4.917 min Scan# 49
Delta R.T. 0.000 min
Lab File: VW027426.D
Acq: 24 Oct 2023 18:57

Instrument :
MSVOA_W
ClientSampleId :
VIBLK549

Tgt Ion: 84 Resp: 26569
Ion Ratio Lower Upper
84 100
86 60.4 41.3 76.7
49 132.7 92.8 172.4

