




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102523\
 Data File : VW027432.D
 Acq On : 25 Oct 2023 10:44
 Operator : SY/MD
 Sample : VW1025SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK589

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/26/2023
 Supervised By :Mahesh Dadoda 10/27/2023

Quant Time: Oct 26 00:49:05 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 26 00:48:25 2023
 Response via : Initial Calibration

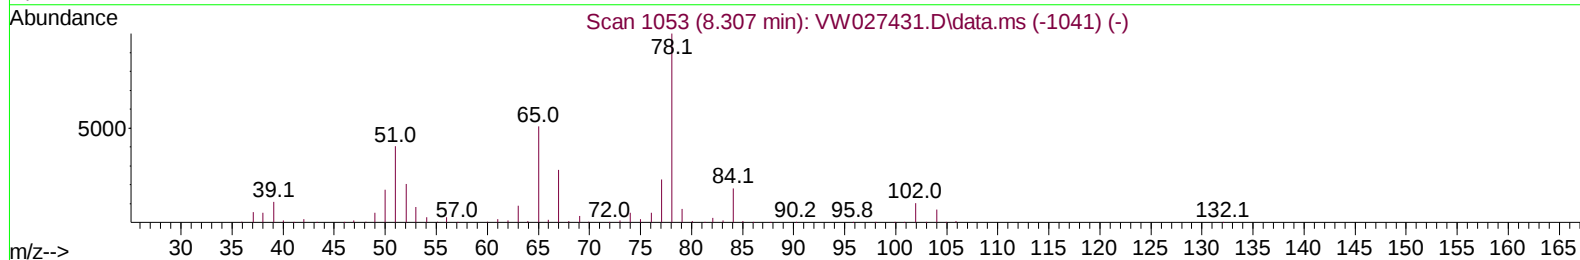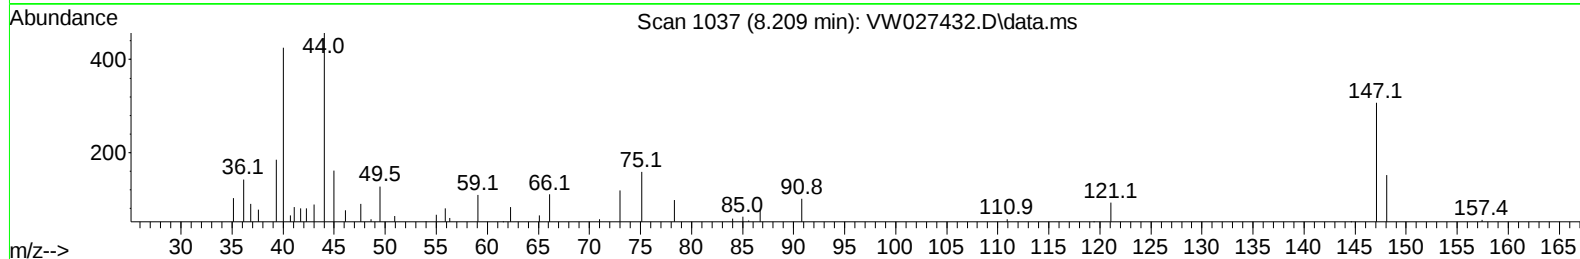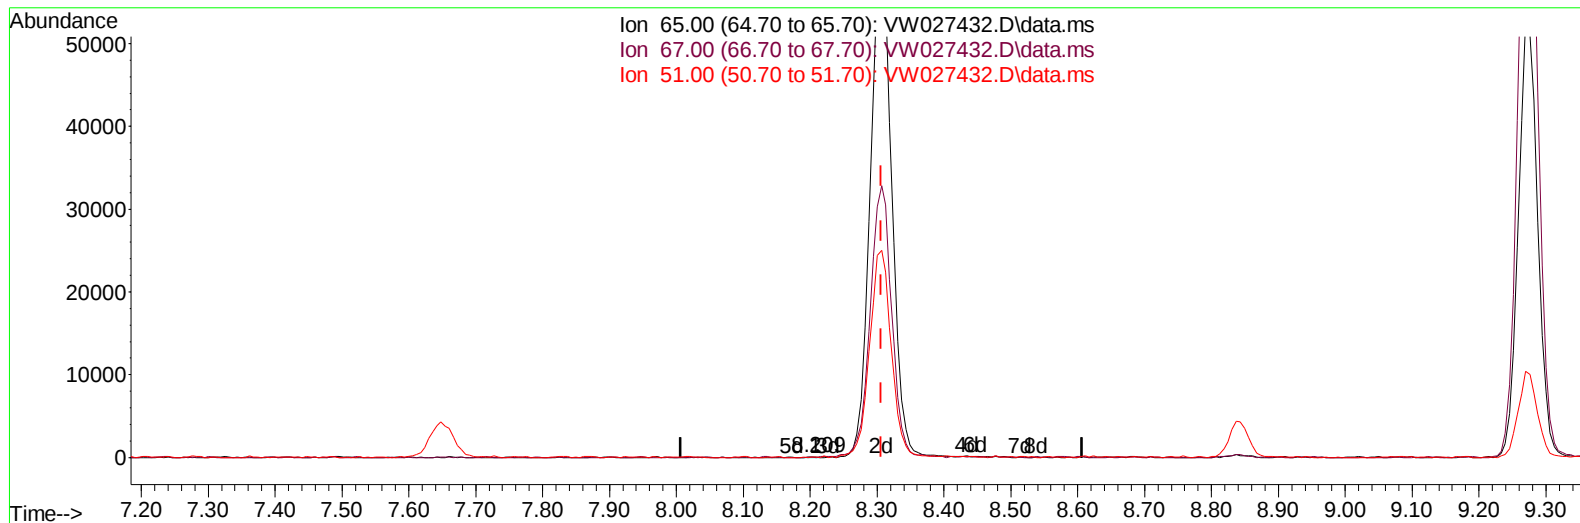

TIC: VW027432.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.209min (-0.098) 0.01 ug/L

response 62

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.00	66.13
51.00	99.60	74.19
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102523\
 Data File : VW027432.D
 Acq On : 25 Oct 2023 10:44
 Operator : SY/MD
 Sample : VW1025SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK589

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/26/2023
 Supervised By :Mahesh Dadoda 10/27/2023

Quant Time: Oct 26 00:49:05 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 26 00:48:25 2023
 Response via : Initial Calibration

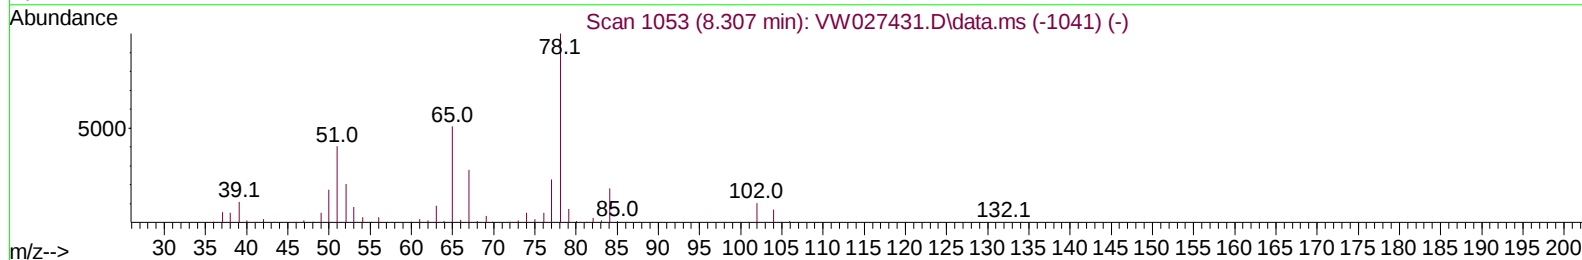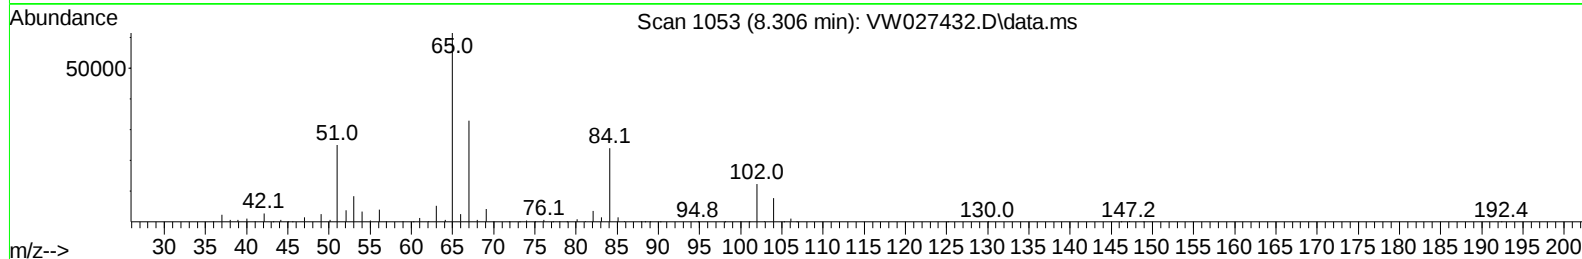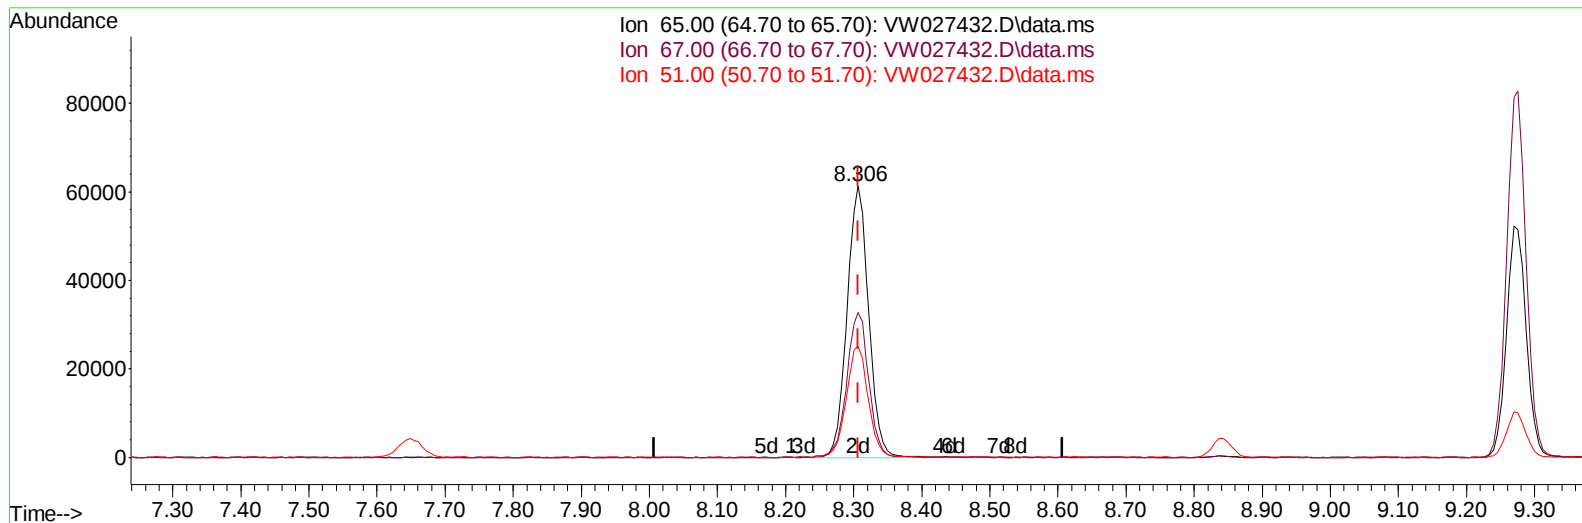

TIC: VW027432.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.306min (-0.000) 21.34 ug/L m

response 134086

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.00	0.03#
51.00	99.60	0.03#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw102523\
 Data File : VW027432.D
 Acq On : 25 Oct 2023 10:44
 Operator : SY/MD
 Sample : VW1025SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK589

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/26/2023
 Supervised By :Mahesh Dadoda 10/27/2023

Quant Time: Oct 26 00:49:05 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 26 00:48:25 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		392365	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		352263	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		179587	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.362	65		107284	17.916	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	71.680%		
7) Chloroethane-d5	2.899	69		88422	20.565	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	82.240%		
11) 1,1-Dichloroethene-d2	4.021	65		57108	19.033	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	76.120%		
21) 2-Butanone-d5	7.075	46		85084	42.749	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	85.500%		
24) Chloroform-d	7.648	84		250747	21.442	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	85.760%		
26) 1,2-Dichloroethane-d4	8.306	65		134086m	21.345	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	85.360%		
32) Benzene-d6	8.276	84		516028	21.652	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	86.600%		
36) 1,2-Dichloropropane-d6	9.276	67		165641	22.754	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	91.000%		
41) Toluene-d8	10.324	98		445750	20.625	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	82.480%		
43) trans-1,3-Dichloroprop...	10.574	79		59914	18.052	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	72.200%		
47) 2-Hexanone-d5	10.922	63		62294	41.361	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	82.720%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		124066	22.843	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	91.360%		
66) 1,2-Dichlorobenzene-d4	13.848	152		138731	21.317	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	85.280%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102523\
Data File : VW027432.D
Acq On : 25 Oct 2023 10:44
Operator : SY/MD
Sample : VW1025SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK589

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/26/2023
Supervised By :Mahesh Dadoda 10/27/2023

Quant Time: Oct 26 00:49:05 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101123SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 26 00:48:25 2023
Response via : Initial Calibration

