

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102524\
 Data File : VW030775.D
 Acq On : 25 Oct 2024 18:30
 Operator : SY/MD
 Sample : P4493-15
 Misc : 5.79g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 25 23:24:55 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 25 23:19:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	105094	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	99963	25.000	ug/L	# 0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	34037	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	20240	12.252	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	49.000%
7) Chloroethane-d5	2.899	69	23483	18.780	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.120%
11) 1,1-Dichloroethene-d2	4.021	65	8737	12.716	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	50.880%
21) 2-Butanone-d5	7.087	46	13513	45.455	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.900%
24) Chloroform-d	7.654	84	73492	24.453	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.800%
26) 1,2-Dichloroethane-d4	8.477	65	97	0.062	ug/L	0.18
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.240%#
32) Benzene-d6	8.276	84	100701	17.357	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	69.440%
36) 1,2-Dichloropropane-d6	9.276	67	41902	24.606	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	98.440%
41) Toluene-d8	10.325	98	70992	13.404	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	53.600%
43) trans-1,3-Dichloroprop...	10.581	79	12718	17.836	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	71.360%
47) 2-Hexanone-d5	10.922	63	9806	44.709	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.420%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	36674	29.325	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	117.320%
66) 1,2-Dichlorobenzene-d4	13.848	152	28220	24.504	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.000%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	1133	0.462	ug/L	# 66
48) 2-Hexanone	10.922	43	1799	2.818	ug/L	# 71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102524\
Data File : VW030775.D
Acq On : 25 Oct 2024 18:30
Operator : SY/MD
Sample : P4493-15
Misc : 5.79g/10mL/MSVOA_W/SOIL/A
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Oct 25 23:24:55 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 25 23:19:25 2024
Response via : Initial Calibration




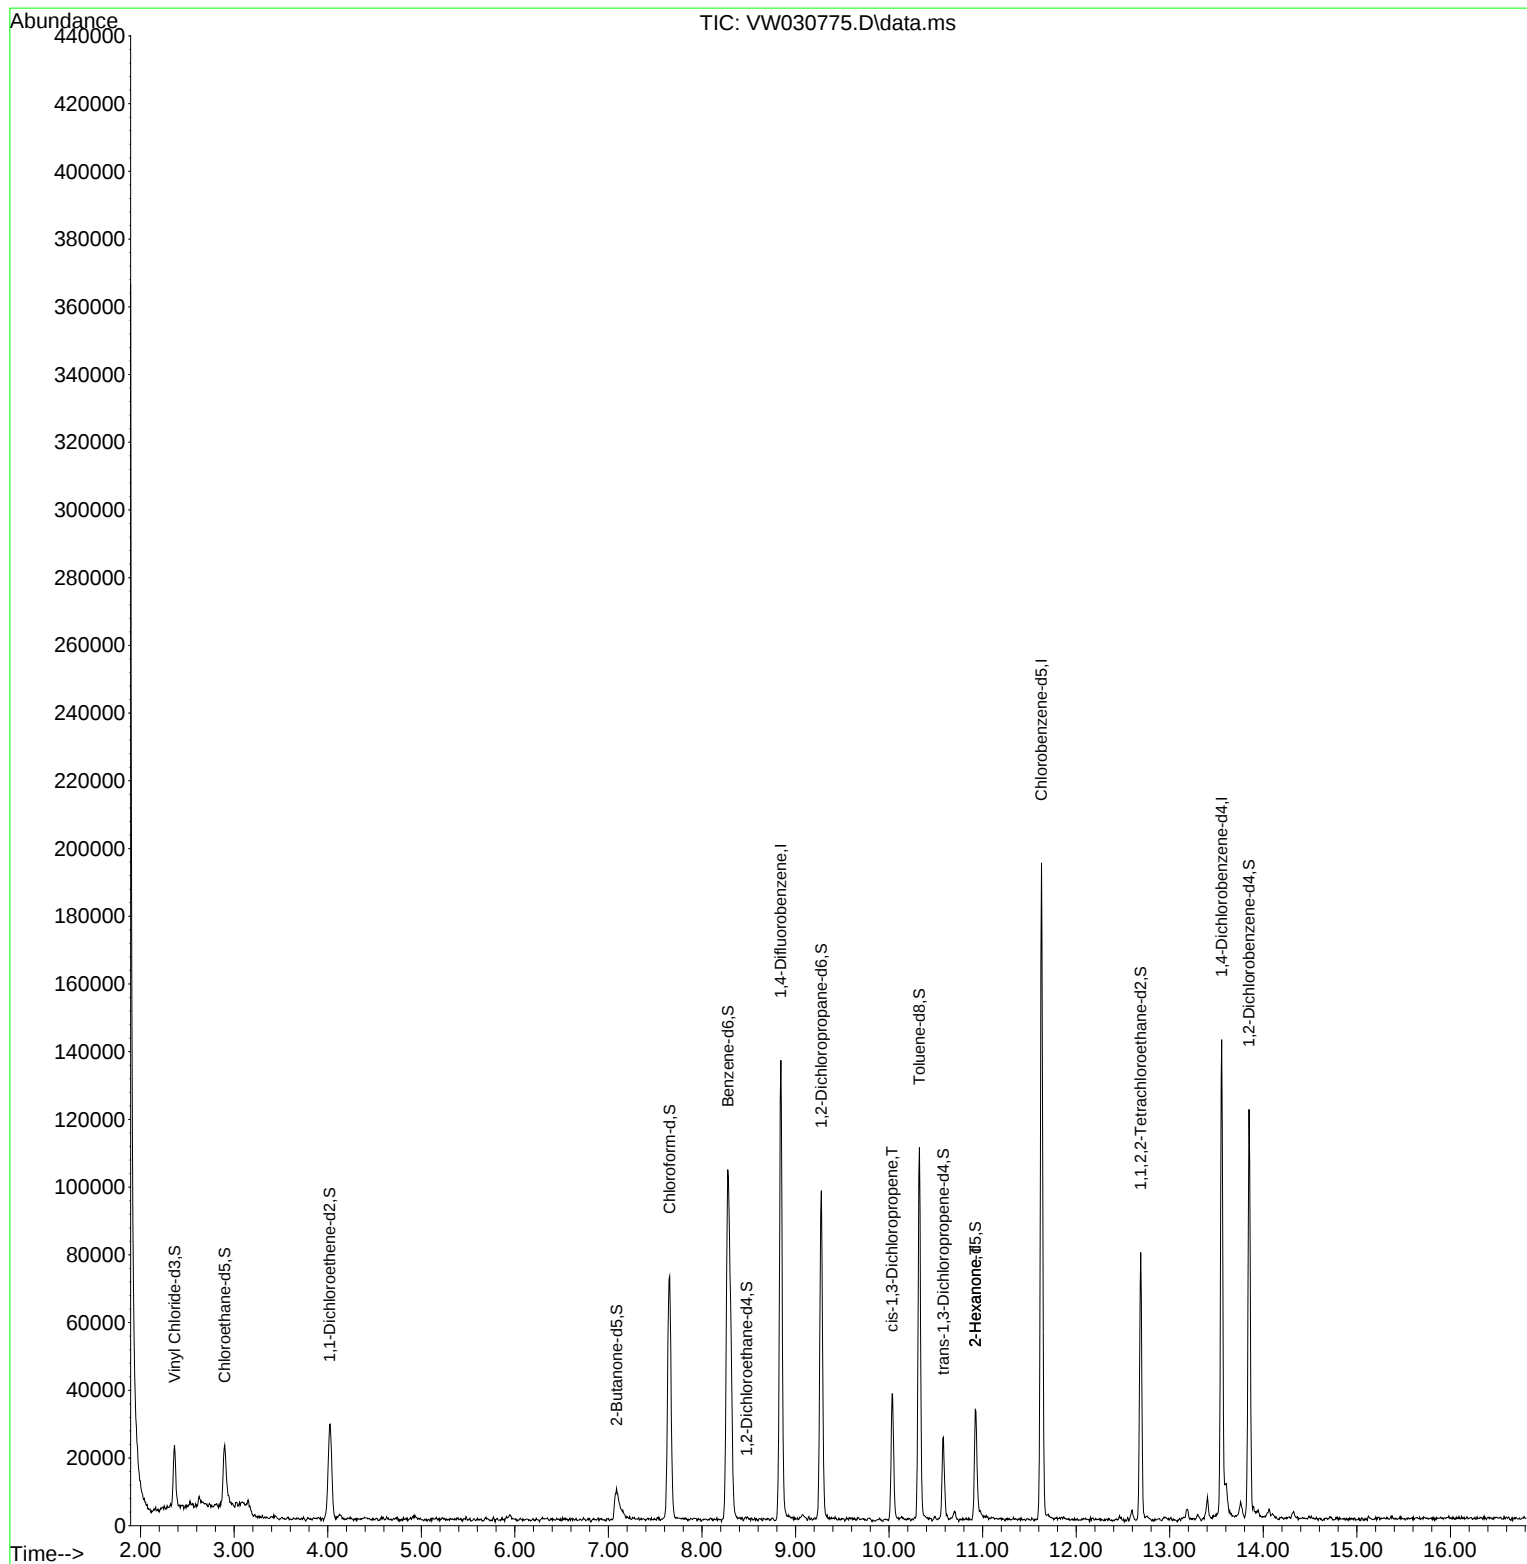


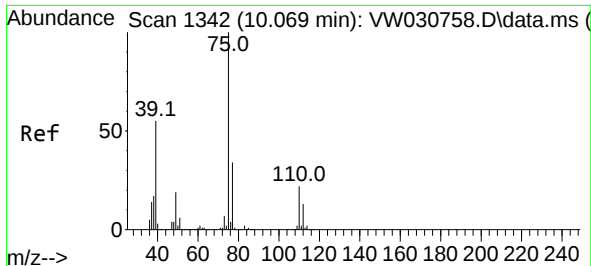

#39
cis-1,3-Dichloropropene
Concen: 0.462 ug/L
RT: 10.032 min Scan# 1133
Delta R.T. -0.037 min
Lab File: VW030775.D
Acq: 25 Oct 2024 18:30

Instrument :
MSVOA_W
ClientSampleId :

Tgt Ion: 75 Resp: 1133
Ion Ratio Lower Upper
75 100
77 48.8 21.1 39.1#

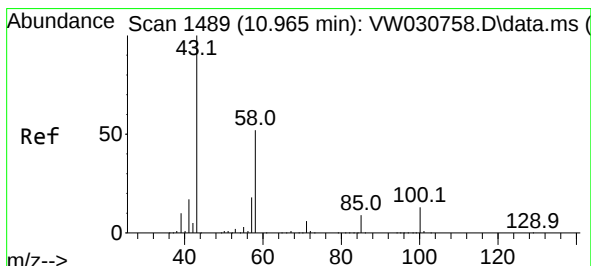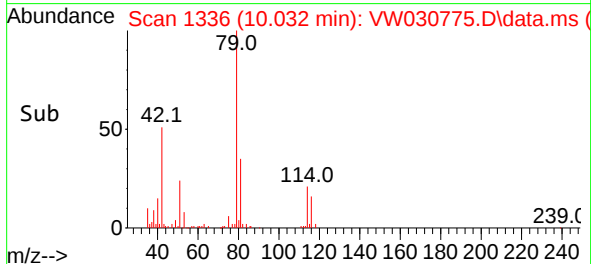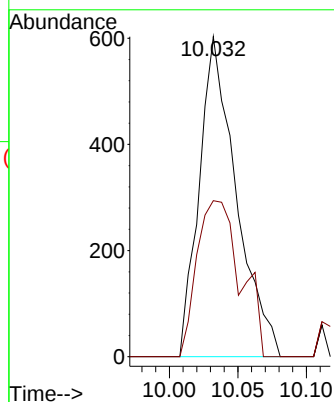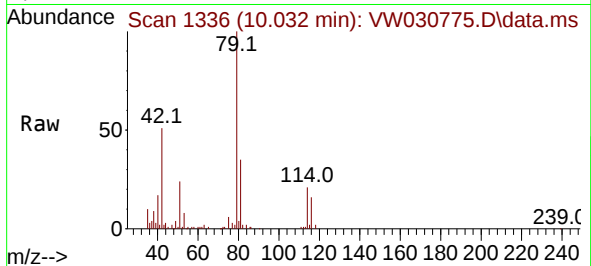

#48
2-Hexanone
Concen: 2.818 ug/L
RT: 10.922 min Scan# 1482
Delta R.T. -0.043 min
Lab File: VW030775.D
Acq: 25 Oct 2024 18:30

Tgt Ion: 43 Resp: 1799
Ion Ratio Lower Upper
43 100
58 39.1 44.6 67.0#
57 46.6 15.8 23.8#
100 9.8 10.2 15.2#

