


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102524\
 Data File : VW030759.D
 Acq On : 25 Oct 2024 11:32
 Operator : SY/MD
 Sample : VW1025SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK582

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
 Yesilyurt
 10/28/2024
 Supervised By :Mahesh
 Dadoda
 10/28/2024

Quant Time: Oct 25 23:20:21 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 25 23:19:25 2024
 Response via : Initial Calibration

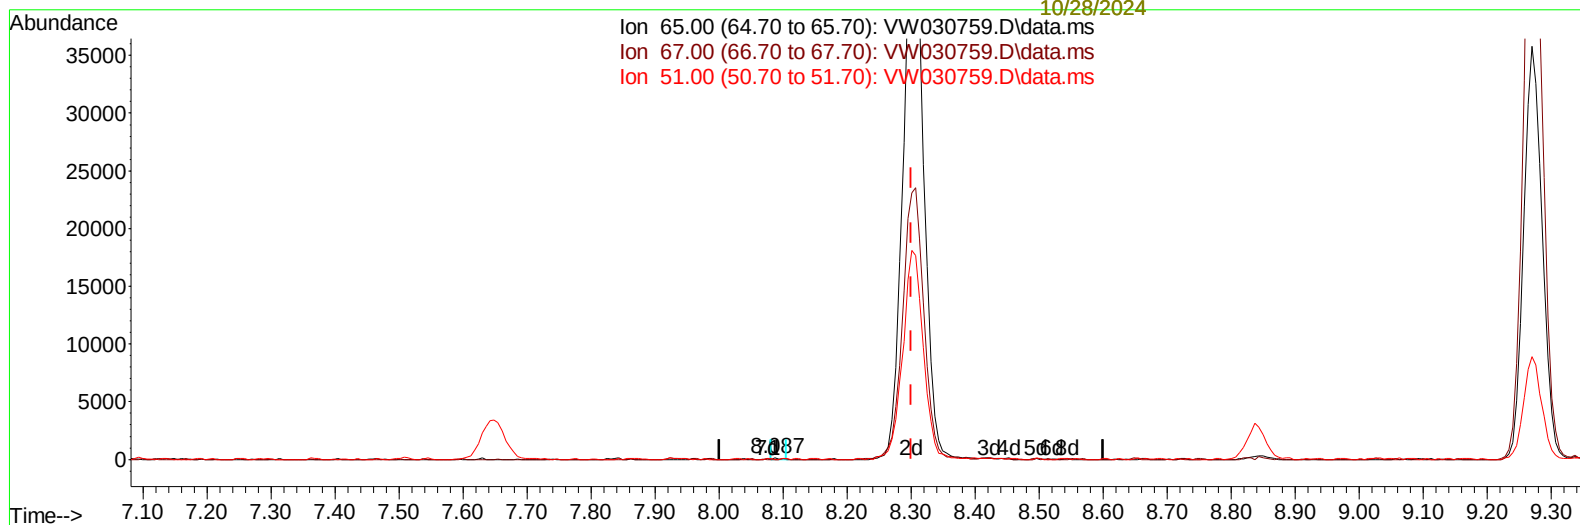




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102524\
Data File : VW030759.D
Acq On : 25 Oct 2024 11:32
Operator : SY/MD
Sample : VW1025SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK582

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
Yesilyurt
10/28/2024
Supervised By :Mahesh
Dadoda
10/28/2024

Quant Time: Oct 25 23:20:21 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 25 23:19:25 2024
Response via : Initial Calibration

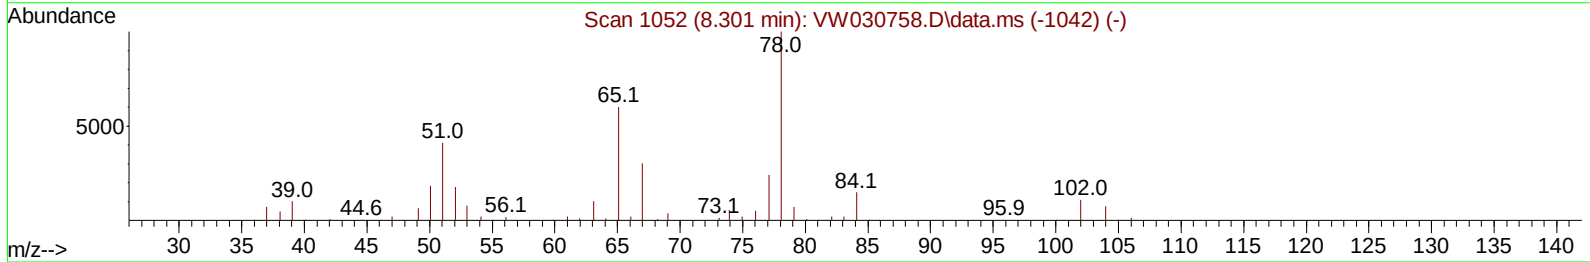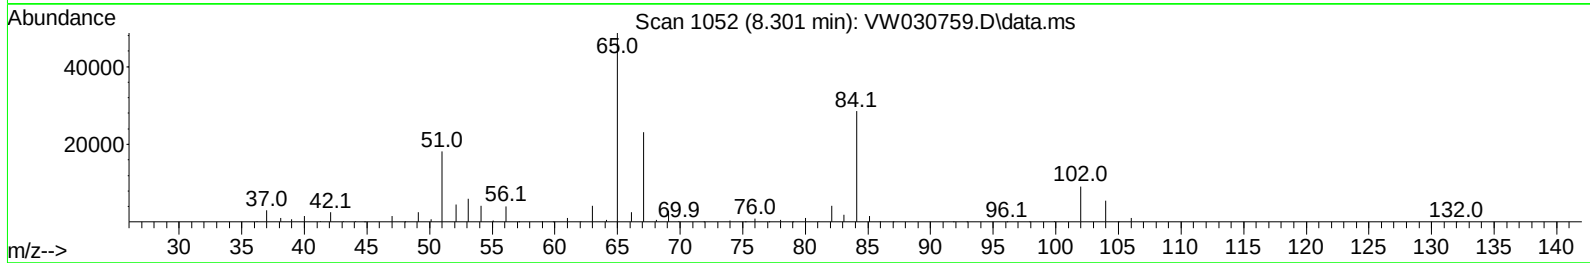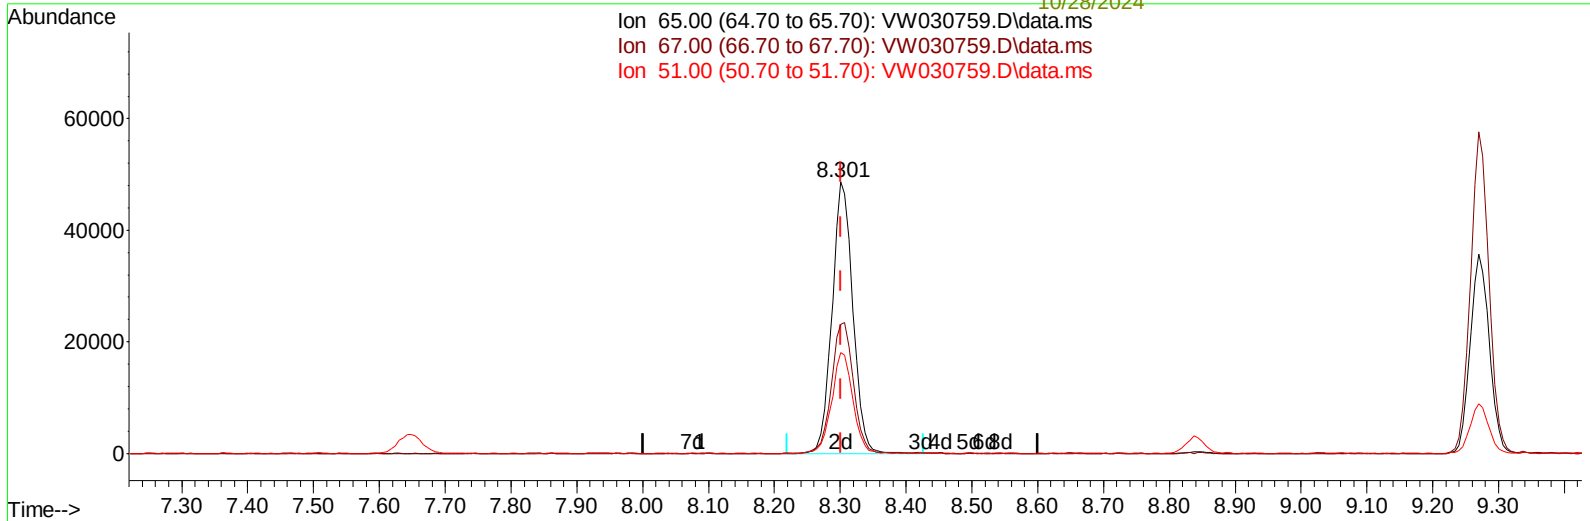

TIC: VW030759.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.301min (-0.000) 28.09 ug/L m

response 106589

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.90	0.05#
51.00	109.40	0.06#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw102524\
 Data File : VW030759.D
 Acq On : 25 Oct 2024 11:32
 Operator : SY/MD
 Sample : VW1025SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK582

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
 Yesilyurt
 10/28/2024
 Supervised By :Mahesh
 Dadoda
 10/28/2024

Quant Time: Oct 25 23:20:21 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 25 23:19:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	255161	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	239882	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	109304	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	106746	26.615	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	106.440%	
7) Chloroethane-d5	2.899	69	88879	29.275	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	117.120%	
11) 1,1-Dichloroethene-d2	4.015	65	43698	26.195	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	104.800%	
21) 2-Butanone-d5	7.075	46	37274	51.642	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	103.280%	
24) Chloroform-d	7.648	84	195098	26.736	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	106.960%	
26) 1,2-Dichloroethane-d4	8.301	65	106589m	28.090	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	112.360%	
32) Benzene-d6	8.270	84	378971	27.220	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	108.880%	
36) 1,2-Dichloropropane-d6	9.270	67	112481	27.525	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	110.120%	
41) Toluene-d8	10.319	98	348462	27.417	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	109.680%	
43) trans-1,3-Dichloroprop...	10.575	79	44683	26.113	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	104.440%	
47) 2-Hexanone-d5	10.922	63	29198	55.474	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	110.940%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	80423	26.798	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	107.200%	
66) 1,2-Dichlorobenzene-d4	13.849	152	104542	28.267	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	113.080%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102524\
Data File : VW030759.D
Acq On : 25 Oct 2024 11:32
Operator : SY/MD
Sample : VW1025SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK582

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
Yesilyurt
10/28/2024
Supervised By :Mahesh
Dadoda
10/28/2024

Quant Time: Oct 25 23:20:21 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 25 23:19:25 2024
Response via : Initial Calibration

