

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102524\
 Data File : VW030768.D
 Acq On : 25 Oct 2024 15:42
 Operator : SY/MD
 Sample : VIBLK560
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK560

Quant Time: Oct 25 23:23:03 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 25 23:19:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	237865	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	225694	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	105326	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	42800	11.447	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	45.800%
7) Chloroethane-d5	2.905	69	42437	14.994	ug/L	0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	59.960%
11) 1,1-Dichloroethene-d2	4.021	65	19242	12.374	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	49.480%
21) 2-Butanone-d5	7.075	46	38428	57.112	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	114.220%
24) Chloroform-d	7.648	84	125444	18.441	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	73.760%
26) 1,2-Dichloroethane-d4	8.307	65	70476	19.924	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	79.680%
32) Benzene-d6	8.276	84	203217	15.514	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	62.040%
36) 1,2-Dichloropropane-d6	9.276	67	72826	18.942	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	75.760%
41) Toluene-d8	10.324	98	167738	14.027	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	56.120%
43) trans-1,3-Dichloroprop...	10.581	79	25683	15.953	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	63.800%
47) 2-Hexanone-d5	10.922	63	27007	54.537	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	109.080%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	72250	25.588	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	102.360%
66) 1,2-Dichlorobenzene-d4	13.848	152	72139	20.242	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	80.960%
Target Compounds						Qvalue
16) Methylene chloride	4.923	84	9834	2.735	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102524\
Data File : VW030768.D
Acq On : 25 Oct 2024 15:42
Operator : SY/MD
Sample : VIBLK560
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK560


Quant Time: Oct 25 23:23:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 25 23:19:25 2024
Response via : Initial Calibration

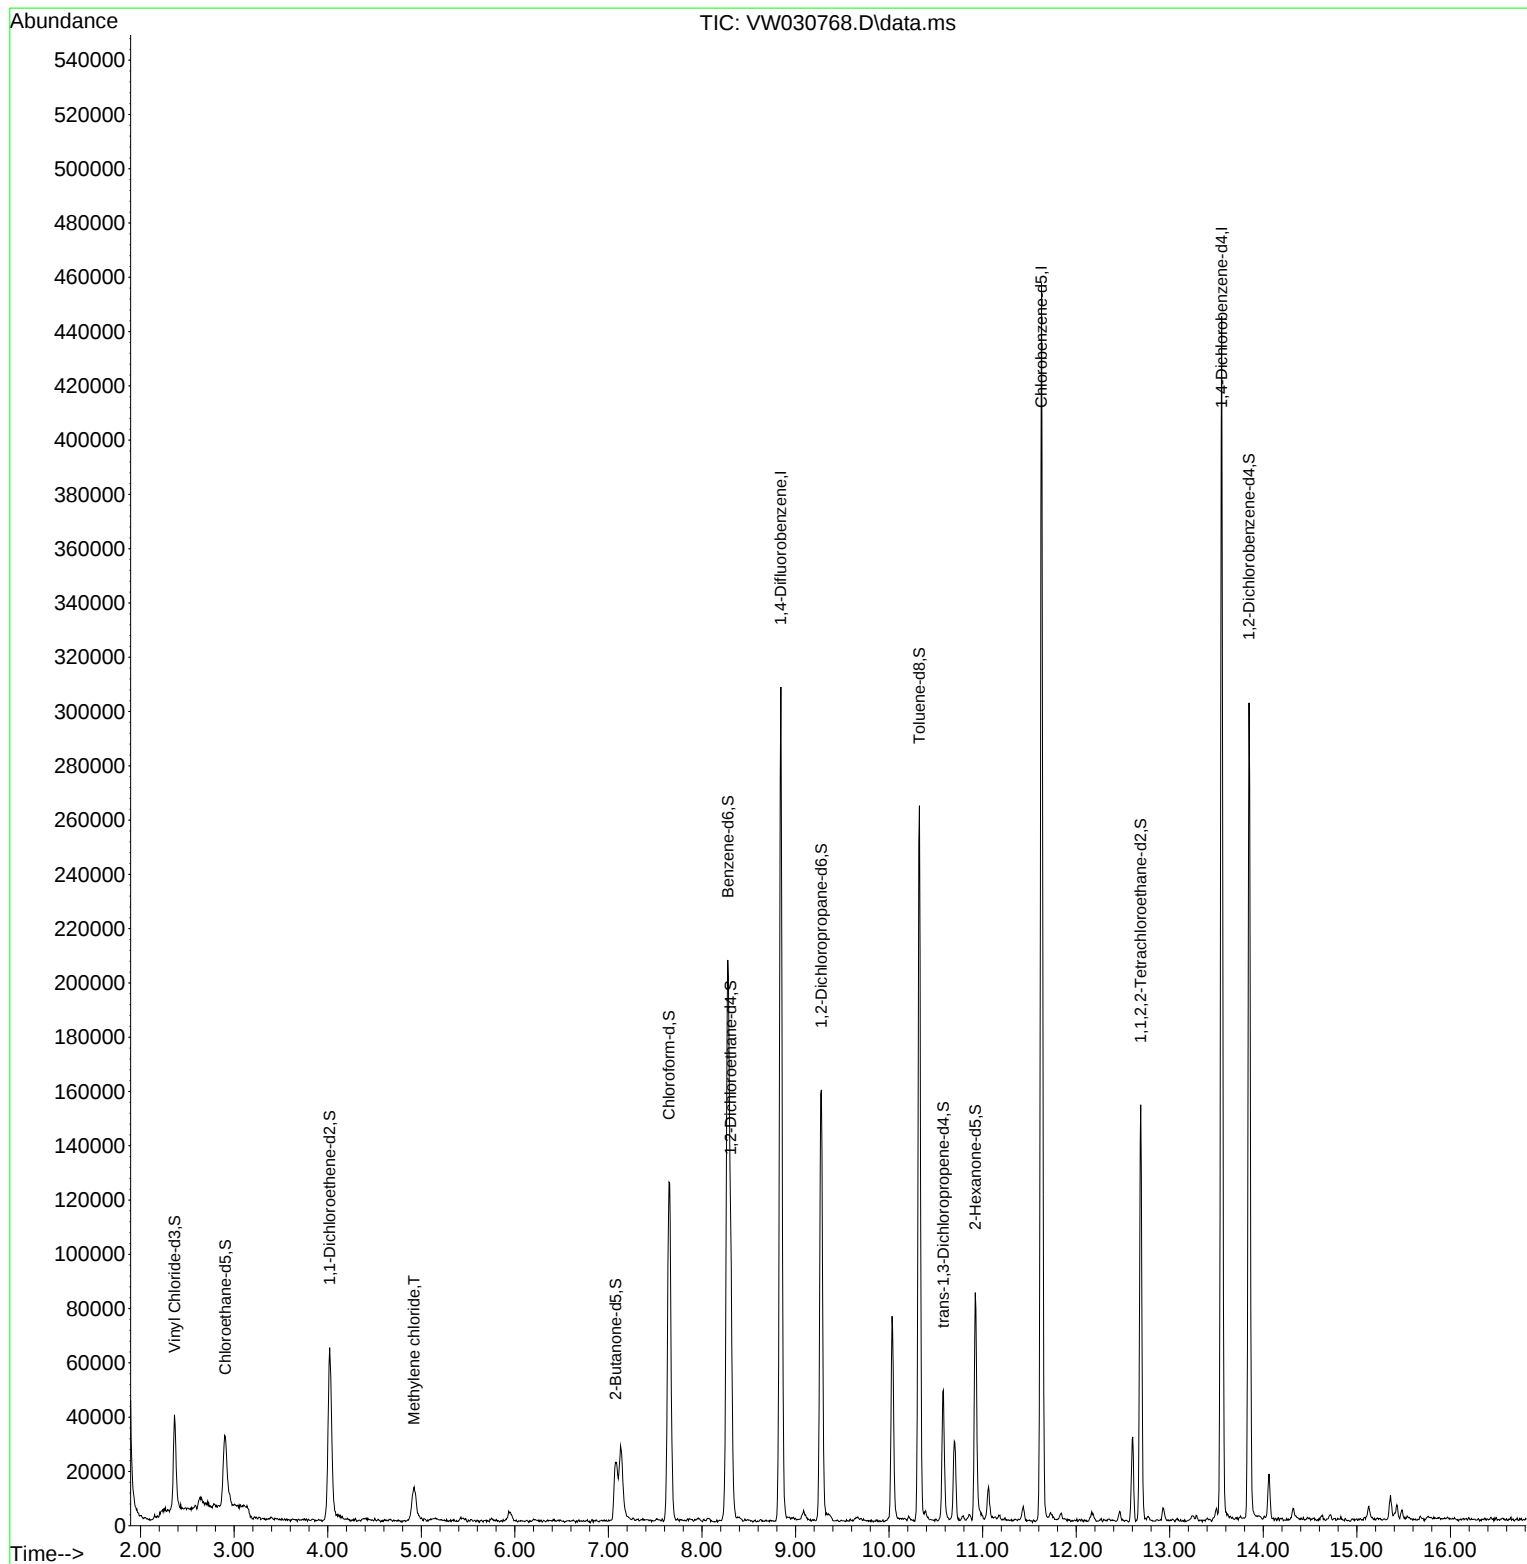

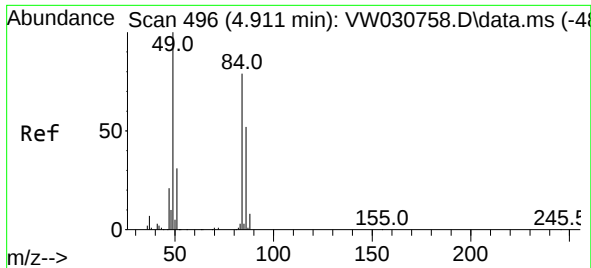

#16
Methylene chloride
Concen: 2.735 ug/L
RT: 4.923 min Scan# 49
Delta R.T. 0.012 min
Lab File: VW030768.D
Acq: 25 Oct 2024 15:42

Instrument :
MSVOA_W
ClientSampleId :
VIBLK560

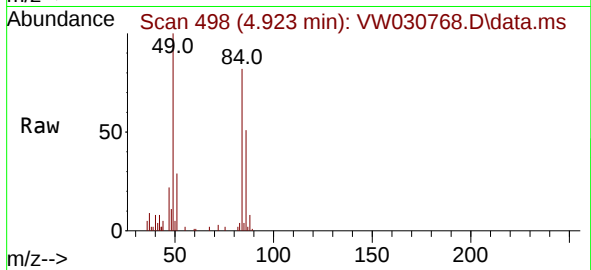

Tgt Ion: 84 Resp: 9834

Ion	Ratio	Lower	Upper
84	100		
86	61.4	43.8	81.3
49	121.3	88.3	164.1

