

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102618\
 Data File : VW006360.D
 Acq On : 25 Oct 2018 13:21
 Operator : SY/AP
 Sample : J5635-12
 Misc : 5.79G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A40J5

Quant Time: Oct 26 04:27:43 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100918S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 26 04:05:39 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	371309	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	322592	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	139767	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	73305	17.51	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.04%
7) Chloroethane-d5	2.90	69	73449	20.38	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.52%
10) 1,1-Dichloroethene-d2	4.01	63	118815	14.78	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	59.12%
20) 2-Butanone-d5	7.09	46	46768	33.69	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	67.38%
24) Chloroform-d	7.65	84	186654	23.21	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.84%
26) 1,2-Dichloroethane-d4	8.31	65	109199	24.54	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.16%
29) Benzene-d6	8.28	84	364457	24.88	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	99.52%
33) 1,2-Dichloropropane-d6	9.28	67	110326	24.96	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.84%
37) Toluene-d8	10.33	98	344877	23.55	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	94.20%
38) trans-1,3-Dichloropropene-	10.58	79	40773	18.98	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	75.92%
39) 2-Hexanone-d5	10.93	63	37957	35.54	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	71.08%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	97848	22.76	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	91.04%
61) 1,2-Dichlorobenzene-d4	13.86	152	116137	24.24	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.96%


Target Compounds					Ovalue
13) Acetone	4.15	43	6351	4.529 ug/L	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW102618\
Data File : VW006360.D
Acq On : 25 Oct 2018 13:21
Operator : SY/AP
Sample : J5635-12
Misc : 5.79G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A40J5

Quant Time: Oct 26 04:27:43 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100918S.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 26 04:05:39 2018
Response via : Initial Calibration

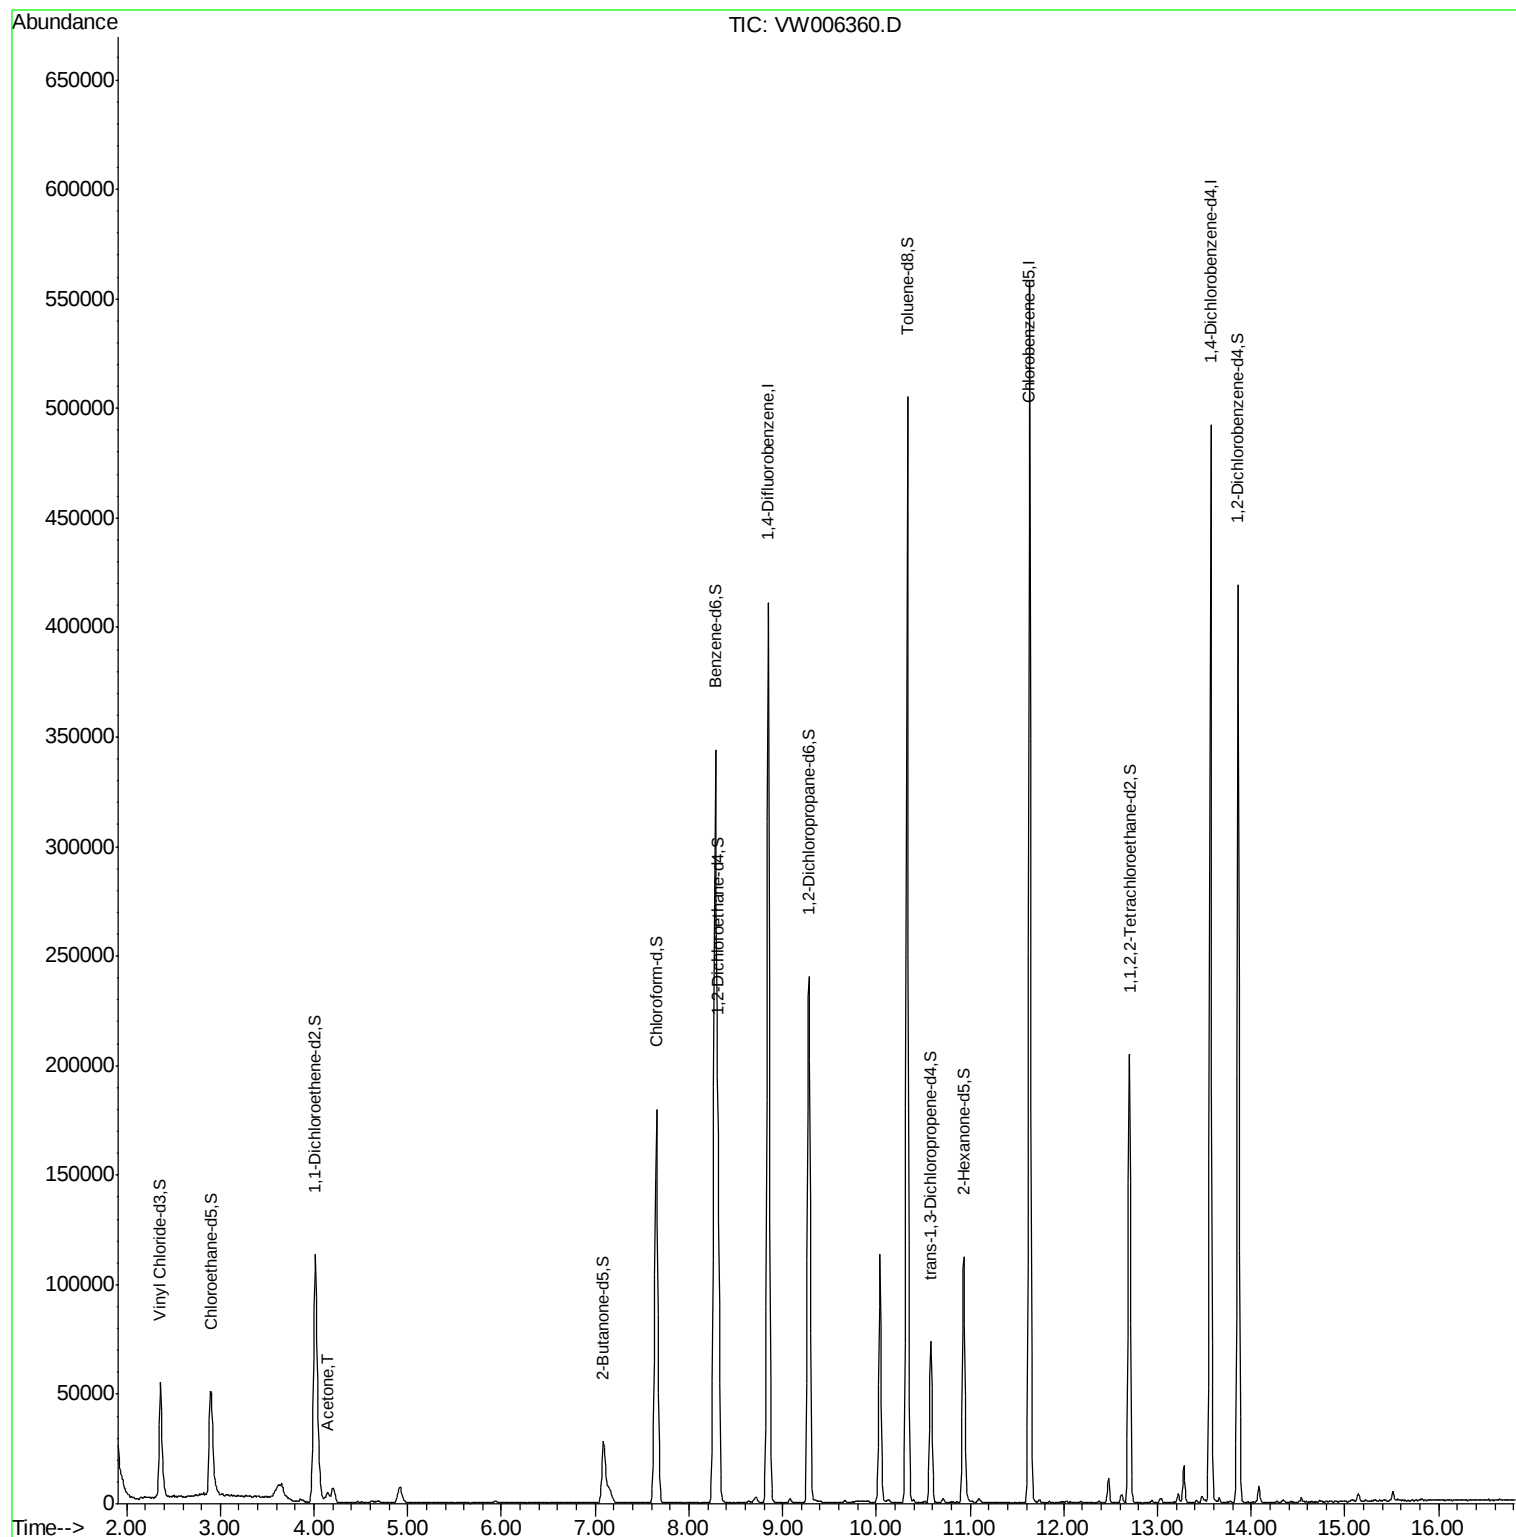

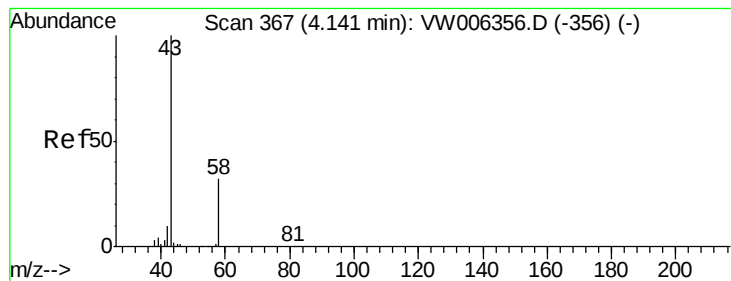

#13

Acetone

Concen: 4.529 ug/L

RT: 4.15 min Scan# 368

Delta R.T. 0.01 min

Lab File: VW006360.D

Acq: 25 Oct 2018 13:21

Instrument :
MSVOA_W
ClientSampleId :
A40J5

Tot Ion: 43 Resp: 6351

Ion Ratio Lower Upper

43 100

58 17.3 0.0 61.2

