

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102618\
 Data File : VW006367.D
 Acq On : 25 Oct 2018 17:06
 Operator : SY/AP
 Sample : J5657-08
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A40B2

Quant Time: Oct 26 05:02:50 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100918S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 26 04:05:39 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	408948	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	382145	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	202076	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	77559	16.82	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	67.28%
7) Chloroethane-d5	2.90	69	79297	19.98	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.92%
10) 1,1-Dichloroethene-d2	4.01	63	126830	14.32	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.28%
20) 2-Butanone-d5	7.09	46	64048	41.90	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	83.80%
24) Chloroform-d	7.65	84	197906	22.34	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.36%
26) 1,2-Dichloroethane-d4	8.31	65	114154	23.29	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	93.16%
29) Benzene-d6	8.27	84	386783	22.29	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	89.16%
33) 1,2-Dichloropropane-d6	9.27	67	115197	22.00	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	88.00%
37) Toluene-d8	10.33	98	376202	21.68	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	86.72%
38) trans-1,3-Dichloropropene-	10.58	79	47387	18.62	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	74.48%
39) 2-Hexanone-d5	10.93	63	53166	42.02	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	84.04%
48) 1,1,2,2-Tetrachloroethane-	12.70	84	115960	22.77	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	91.08%
61) 1,2-Dichlorobenzene-d4	13.86	152	166193	24.00	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.00%


Target Compounds					Ovalue
13) Acetone	4.15	43	39271	25.428 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW102618\
Data File : VW006367.D
Acq On : 25 Oct 2018 17:06
Operator : SY/AP
Sample : J5657-08
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A40B2

Quant Time: Oct 26 05:02:50 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100918S.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 26 04:05:39 2018
Response via : Initial Calibration

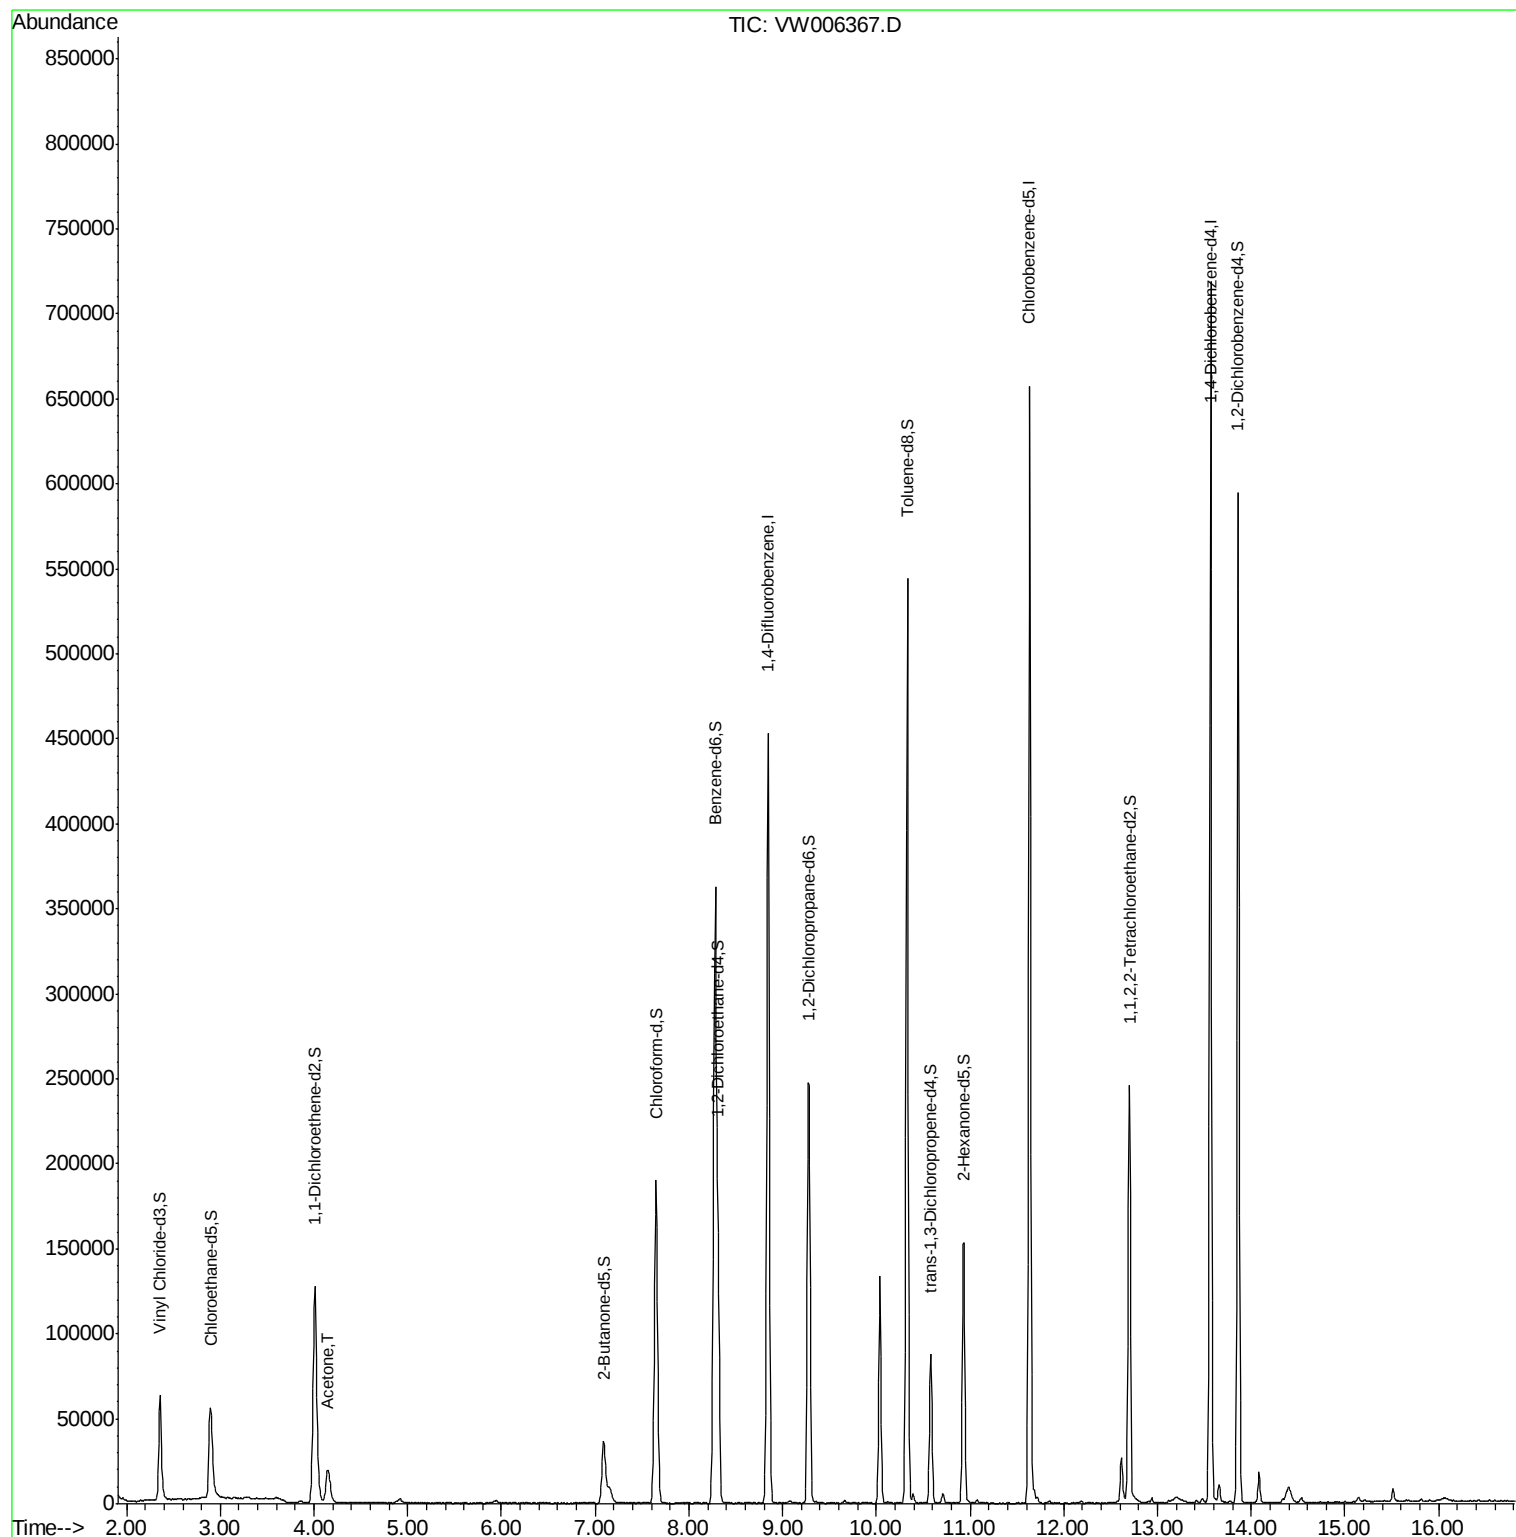

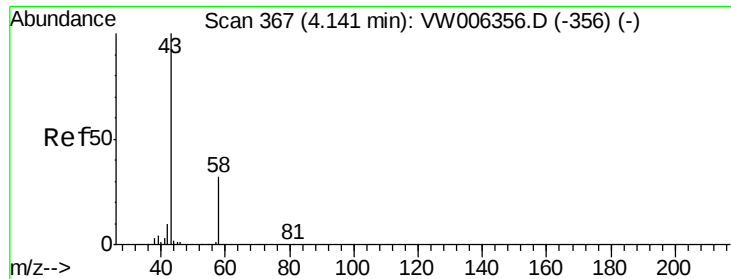

#13
 Acetone
 Concen: 25.428 ug/L
 RT: 4.15 min Scan# 368
 Delta R.T. 0.01 min
 Lab File: VW006367.D
 Acq: 25 Oct 2018 17:06

Instrument :
 MSVOA_W
 ClientSampleId :
 A40B2

Tot Ion: 43 Resp: 39271
 Ion Ratio Lower Upper
 43 100
 58 31.1 0.0 61.2

