

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102618\
 Data File : VW006368.D
 Acq On : 25 Oct 2018 17:32
 Operator : SY/AP
 Sample : J5657-16
 Misc : 5.28G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A40F1

Quant Time: Oct 26 05:04:41 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100918S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 26 04:05:39 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	393109	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	366184	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	195224	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	71394	16.10	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	64.40%
7) Chloroethane-d5	2.90	69	72631	19.03	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.12%
10) 1,1-Dichloroethene-d2	4.01	63	116827	13.72	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	54.88%
20) 2-Butanone-d5	7.09	46	54439	37.05	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	74.10%
24) Chloroform-d	7.65	84	183791	21.58	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.32%
26) 1,2-Dichloroethane-d4	8.31	65	105380	22.37	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	89.48%
29) Benzene-d6	8.28	84	357223	21.49	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	85.96%
33) 1,2-Dichloropropane-d6	9.28	67	108299	21.58	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	86.32%
37) Toluene-d8	10.33	98	351329	21.13	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	84.52%
38) trans-1,3-Dichloropropene-	10.58	79	43408	17.80	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	71.20%
39) 2-Hexanone-d5	10.93	63	45955	37.91	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	75.82%
48) 1,1,2,2-Tetrachloroethane-	12.70	84	104501	21.42	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	85.68%
61) 1,2-Dichlorobenzene-d4	13.86	152	155755	23.28	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	93.12%


Target Compounds					Ovalue
13) Acetone	4.14	43	31213	21.025 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW102618\
Data File : VW006368.D
Acq On : 25 Oct 2018 17:32
Operator : SY/AP
Sample : J5657-16
Misc : 5.28G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
A40F1

Quant Time: Oct 26 05:04:41 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100918S.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 26 04:05:39 2018
Response via : Initial Calibration

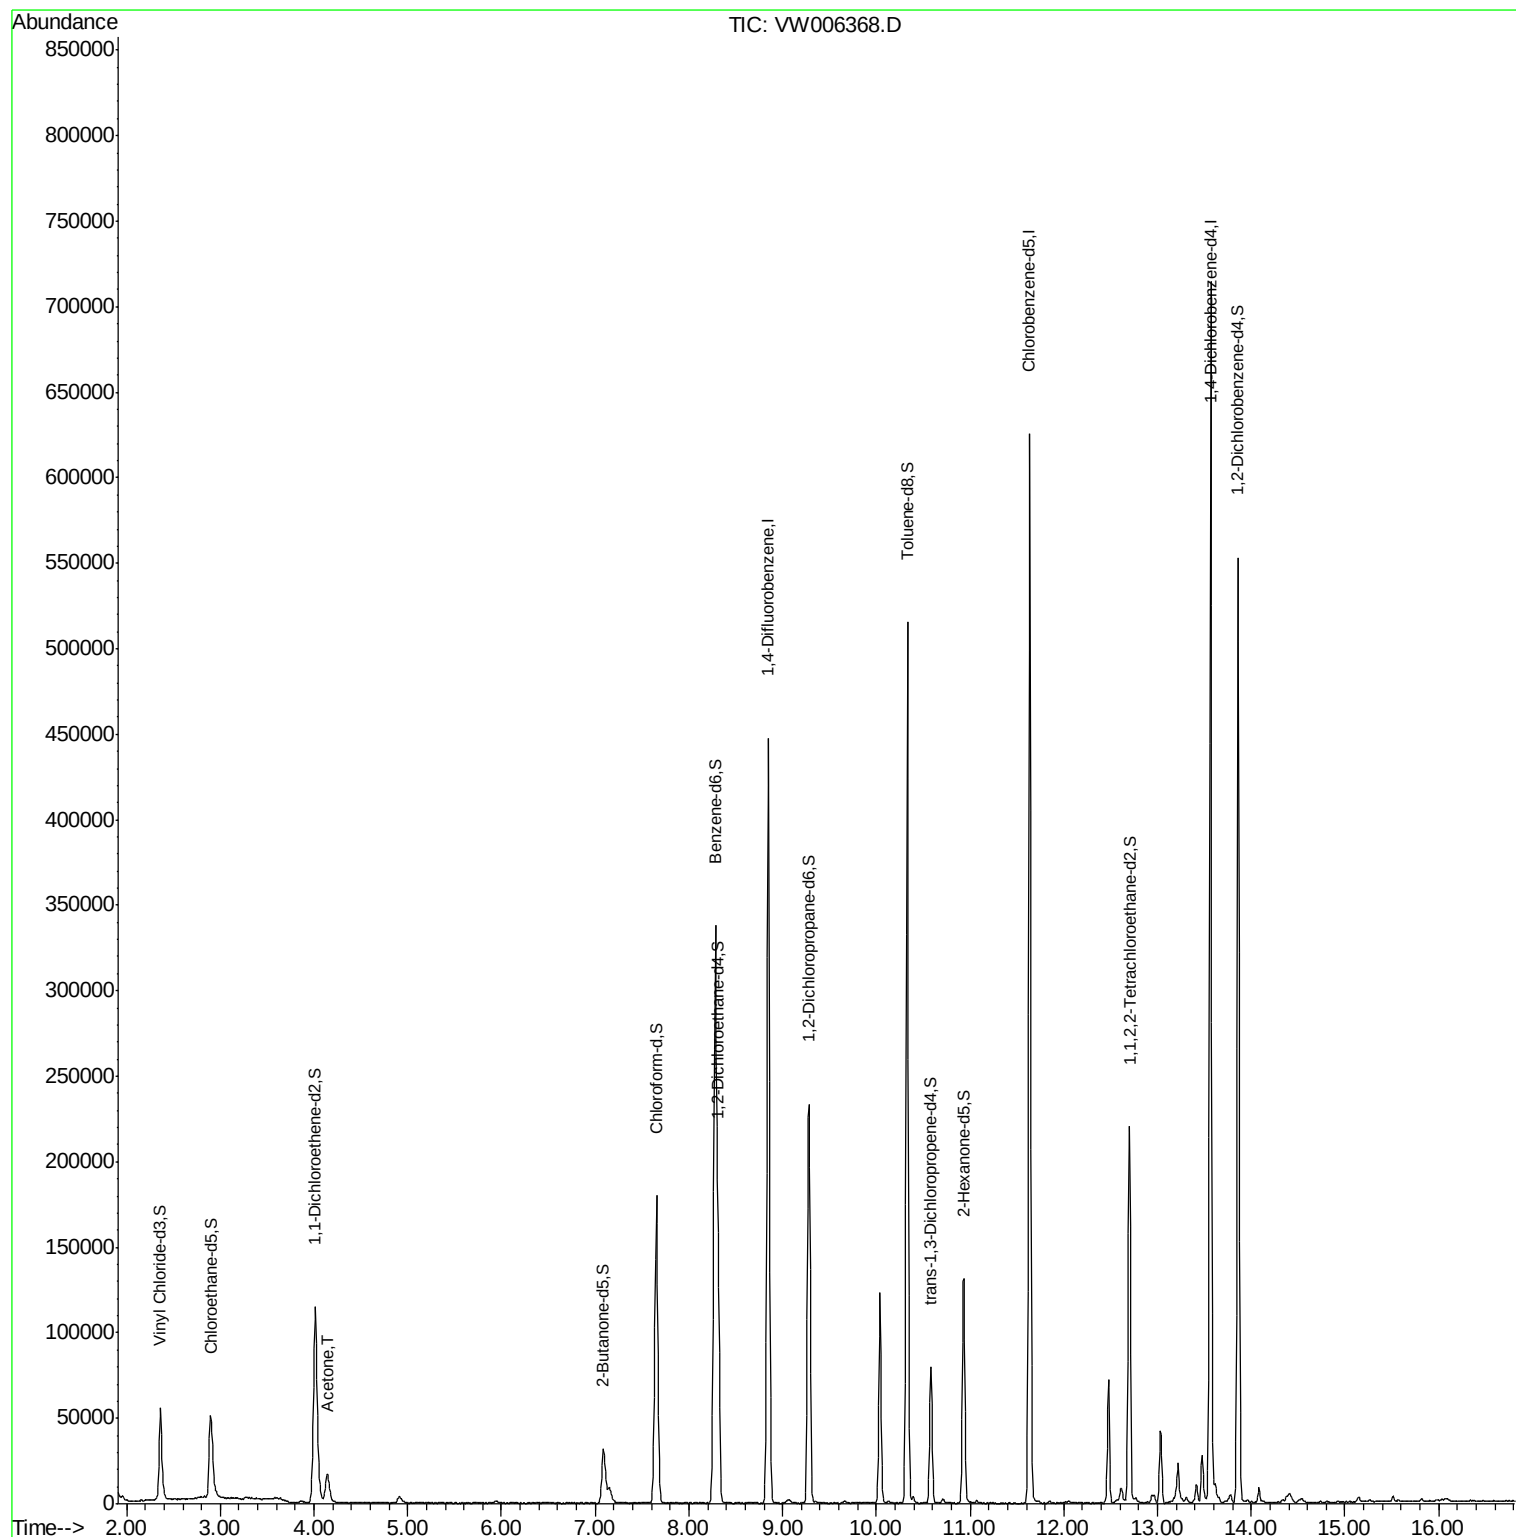

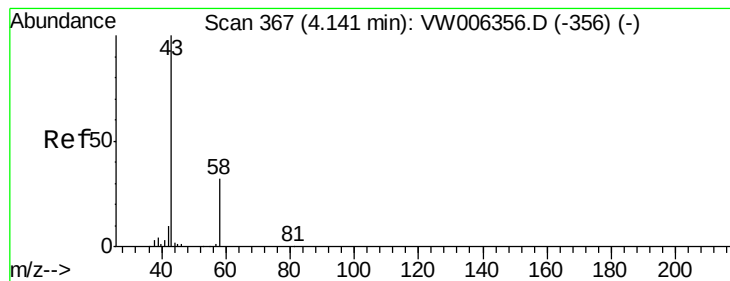

#13
 Acetone
 Concen: 21.025 ug/L
 RT: 4.14 min Scan# 367
 Delta R.T. 0.00 min
 Lab File: VW006368.D
 Acq: 25 Oct 2018 17:32

Instrument :
 MSVOA_W
 ClientSampleId :
 A40F1

Tot Ion: 43 Resp: 31213
 Ion Ratio Lower Upper
 43 100
 58 29.7 0.0 61.2

