

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102618\
 Data File : VW006371.D
 Acq On : 25 Oct 2018 18:49
 Operator : SY/AP
 Sample : J5657-13
 Misc : 4.51G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A40E2

Quant Time: Oct 26 05:09:47 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100918S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 26 04:05:39 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	354290	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	333118	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	174437	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	69420	17.37	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	69.48%
7) Chloroethane-d5	2.90	69	69434	20.19	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.76%
10) 1,1-Dichloroethene-d2	4.01	63	111110	14.48	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.92%
20) 2-Butanone-d5	7.09	46	53221	40.18	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	80.36%
24) Chloroform-d	7.65	84	178161	23.21	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.84%
26) 1,2-Dichloroethane-d4	8.31	65	102311	24.10	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.40%
29) Benzene-d6	8.28	84	345541	22.85	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	91.40%
33) 1,2-Dichloropropane-d6	9.28	67	104768	22.95	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.80%
37) Toluene-d8	10.33	98	339044	22.42	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	89.68%
38) trans-1,3-Dichloropropene-	10.58	79	42977	19.37	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	77.48%
39) 2-Hexanone-d5	10.93	63	44647	40.48	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	80.96%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	99915	22.51	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.04%
61) 1,2-Dichlorobenzene-d4	13.86	152	147282	24.63	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.52%


Target Compounds					Ovalue
13) Acetone	4.14	43	13027	9.736 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW102618\
Data File : VW006371.D
Acq On : 25 Oct 2018 18:49
Operator : SY/AP
Sample : J5657-13
Misc : 4.51G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A40E2

Quant Time: Oct 26 05:09:47 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100918S.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 26 04:05:39 2018
Response via : Initial Calibration

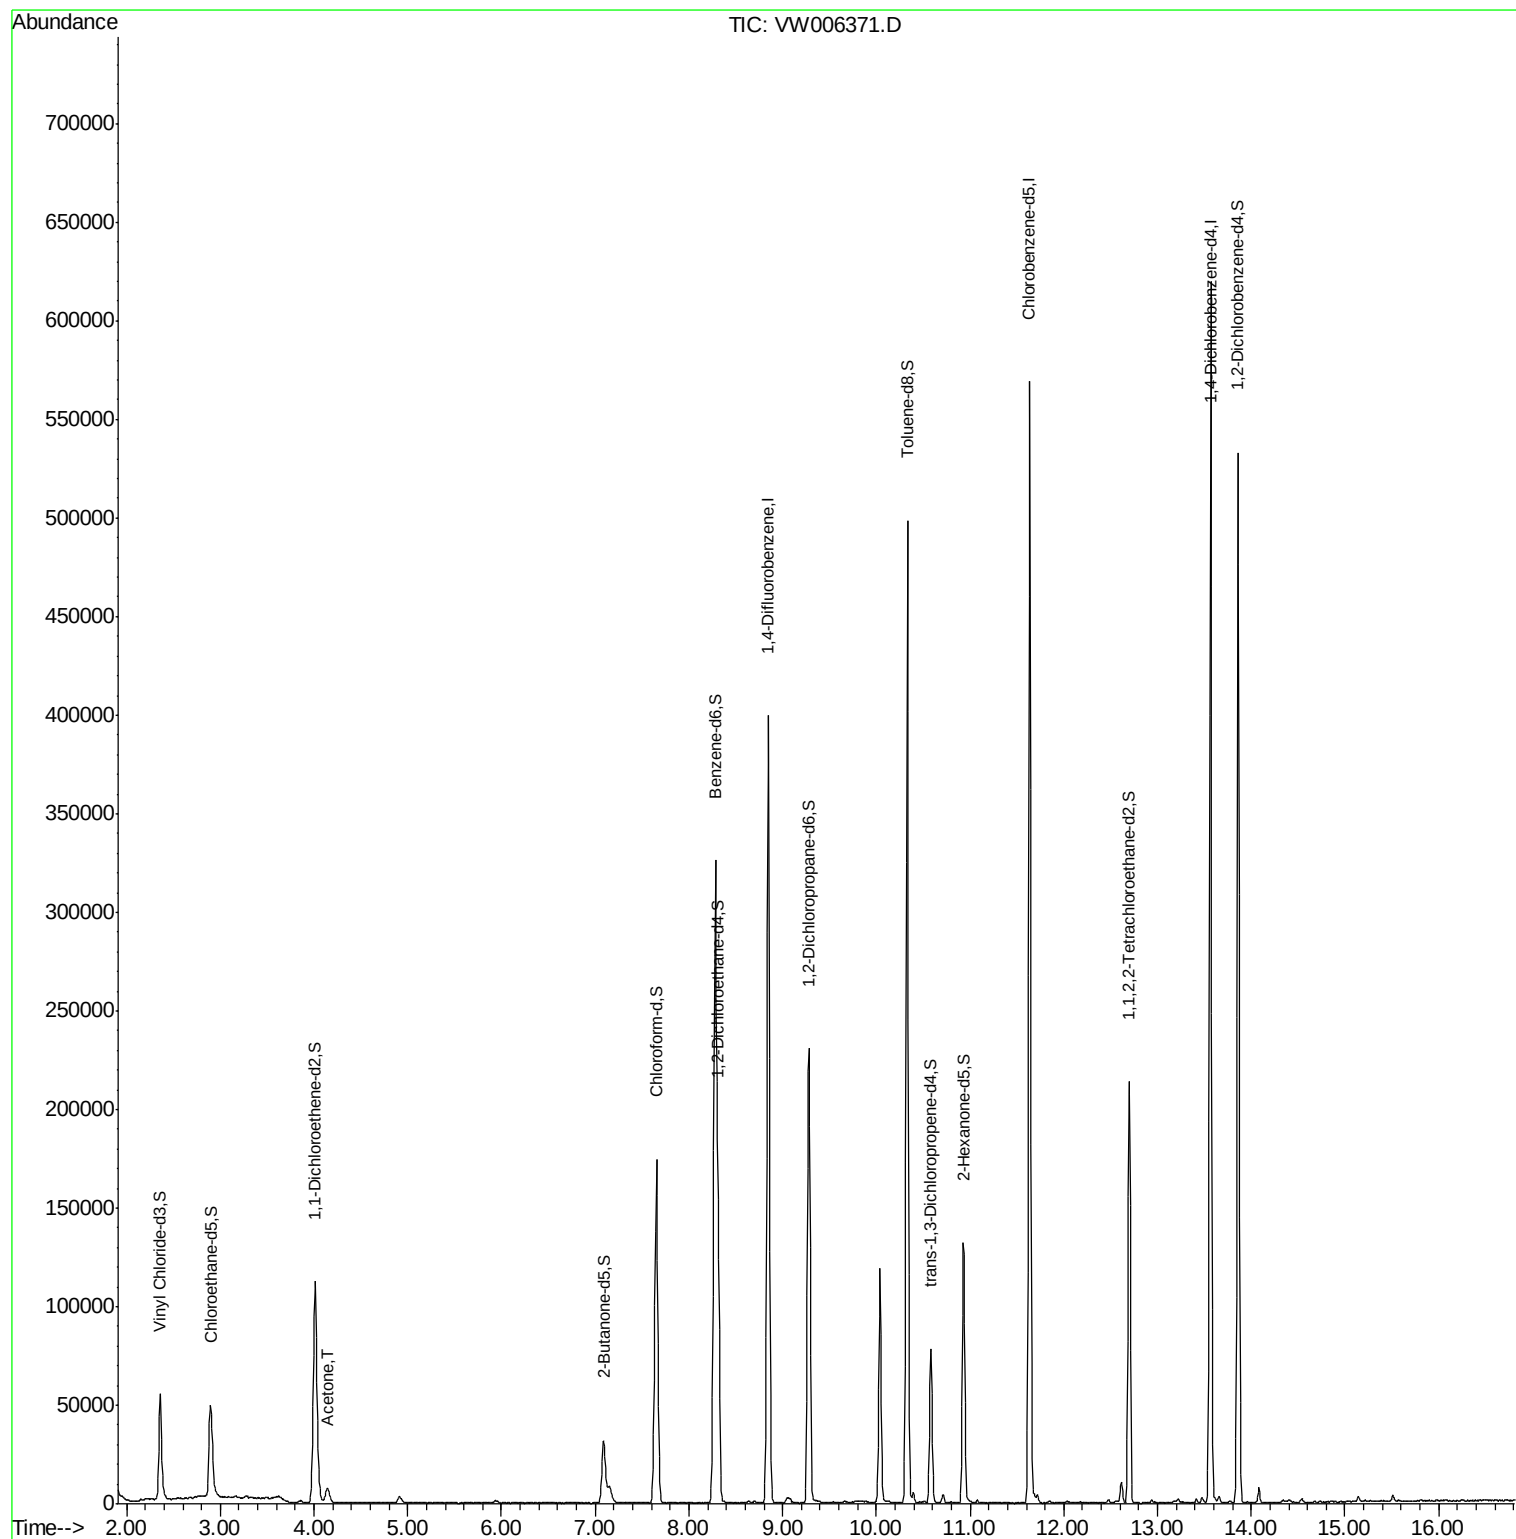

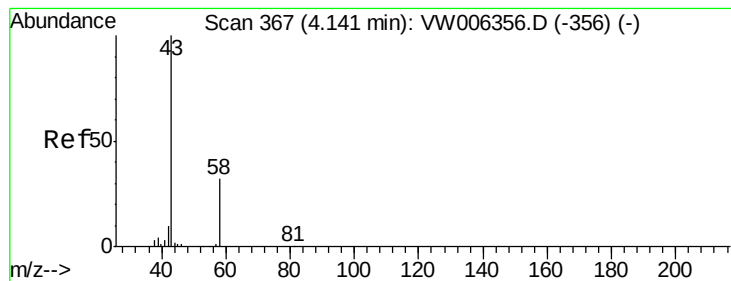

#13

Acetone

Concen: 9.736 ug/L

RT: 4.14 min Scan# 367

Delta R.T. 0.00 min

Lab File: VW006371.D

Acq: 25 Oct 2018 18:49

Instrument :

MSVOA_W

ClientSampleId :

A40E2

Tot Ion: 43 Resp: 13027

Ion Ratio Lower Upper

43 100

58 28.8 0.0 61.2

