

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102618\
 Data File : VW006373.D
 Acq On : 25 Oct 2018 19:41
 Operator : SY/AP
 Sample : VIBLK86
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK86

Quant Time: Oct 26 05:14:03 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100918S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 26 04:05:39 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	362883	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	338679	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	183067	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	60393	14.76	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	59.04%
7) Chloroethane-d5	2.90	69	62012	17.60	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.40%
10) 1,1-Dichloroethene-d2	4.01	63	97284	12.38	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	49.52%
20) 2-Butanone-d5	7.09	46	51557	38.01	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	76.02%
24) Chloroform-d	7.65	84	147766	18.80	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	75.20%
26) 1,2-Dichloroethane-d4	8.31	65	86067	19.79	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	79.16%
29) Benzene-d6	8.28	84	293071	19.06	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	76.24%
33) 1,2-Dichloropropane-d6	9.28	67	86939	18.73	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	74.92%
37) Toluene-d8	10.33	98	283796	18.46	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	73.84%
38) trans-1,3-Dichloropropene-	10.58	79	34184	15.16	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	60.64%
39) 2-Hexanone-d5	10.93	63	42757	38.13	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	76.26%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	90103	19.97	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	79.88%
61) 1,2-Dichlorobenzene-d4	13.86	152	127564	20.33	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	81.32%


Target Compounds					Ovalue
13) Acetone	4.15	43	4785	3.492 ug/L	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW102618\
Data File : VW006373.D
Acq On : 25 Oct 2018 19:41
Operator : SY/AP
Sample : VIBLK86
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK86

Quant Time: Oct 26 05:14:03 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100918S.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 26 04:05:39 2018
Response via : Initial Calibration

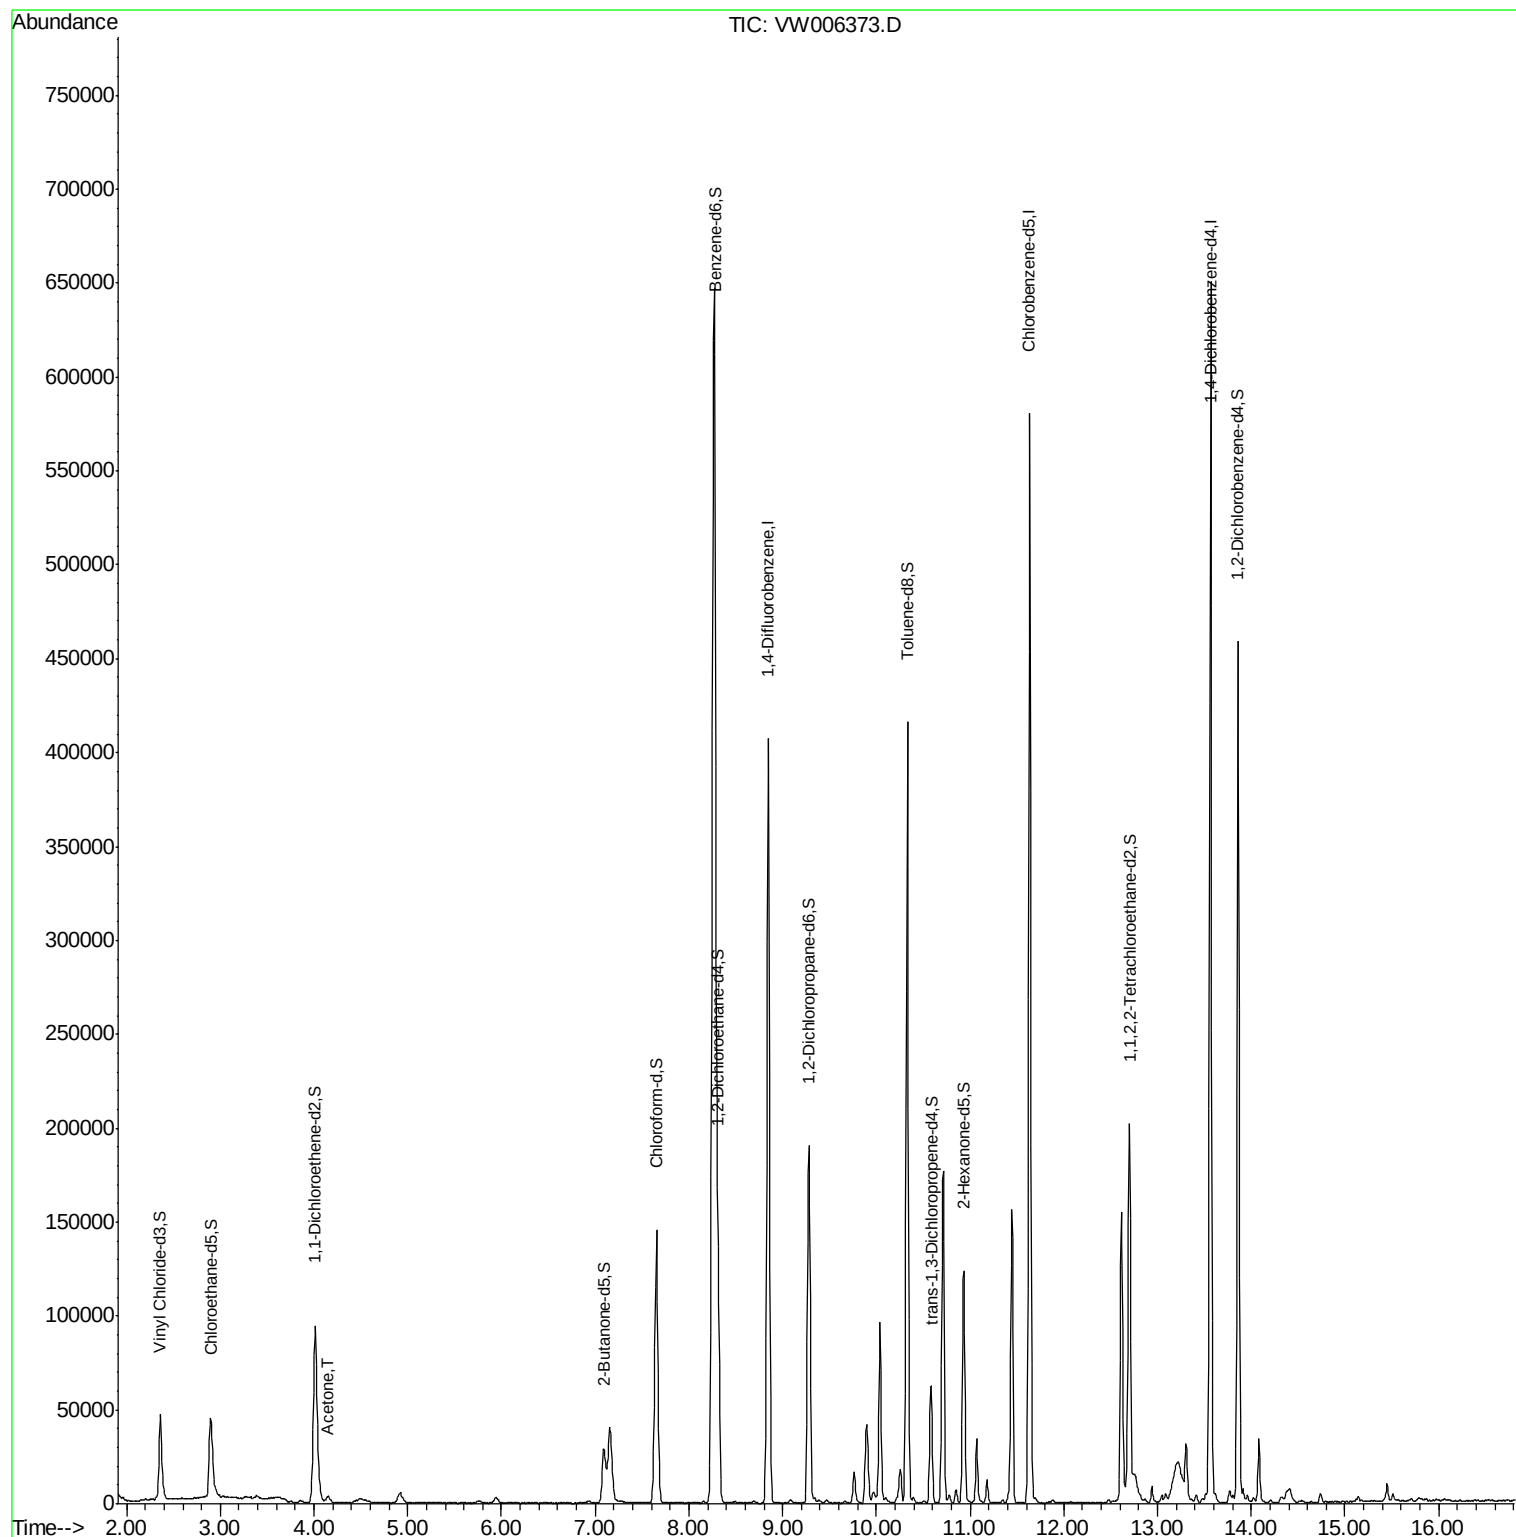

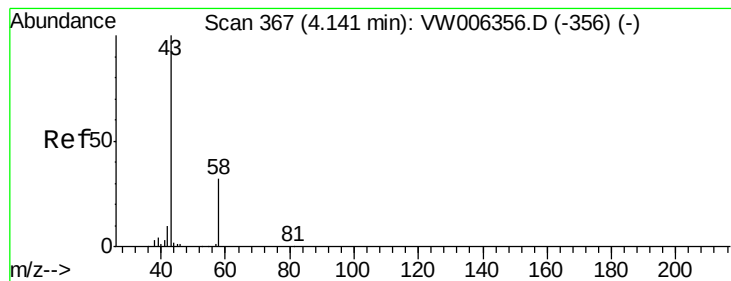

#13
 Acetone
 Concen: 3.492 ug/L
 RT: 4.15 min Scan# 368
 Delta R.T. 0.01 min
 Lab File: VW006373.D
 Acq: 25 Oct 2018 19:41

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK86

Tot Ion: 43 Resp: 4785
 Ion Ratio Lower Upper
 43 100
 58 19.6 0.0 61.2

