

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102824\
 Data File : VW030782.D
 Acq On : 28 Oct 2024 13:15
 Operator : SY/MD
 Sample : VW1028SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 29 01:32:56 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Oct 29 01:29:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	223749	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	209804	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	92894	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	93437	26.567	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	106.280%
7) Chloroethane-d5	2.893	69	80220	30.133	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	120.520%
11) 1,1-Dichloroethene-d2	4.015	65	36956	25.264	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	101.040%
21) 2-Butanone-d5	7.075	46	27102	42.820	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.640%
24) Chloroform-d	7.648	84	169119	26.430	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	105.720%
26) 1,2-Dichloroethane-d4	8.471	65	96	0.029	ug/L	0.17
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.120%#
32) Benzene-d6	8.276	84	326078	26.778	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	107.120%
36) 1,2-Dichloropropane-d6	9.270	67	95025	26.587	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	106.360%
41) Toluene-d8	10.325	98	289762	26.067	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	104.280%
43) trans-1,3-Dichloroprop...	10.575	79	35580	23.774	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	95.080%
47) 2-Hexanone-d5	10.922	63	19129	41.554	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	83.100%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	61963	23.607	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.440%
66) 1,2-Dichlorobenzene-d4	13.848	152	86932	27.658	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	110.640%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	3559	0.692	ug/L #	45


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102824\
Data File : VW030782.D
Acq On : 28 Oct 2024 13:15
Operator : SY/MD
Sample : VW1028SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Oct 29 01:32:56 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Oct 29 01:29:12 2024
Response via : Initial Calibration

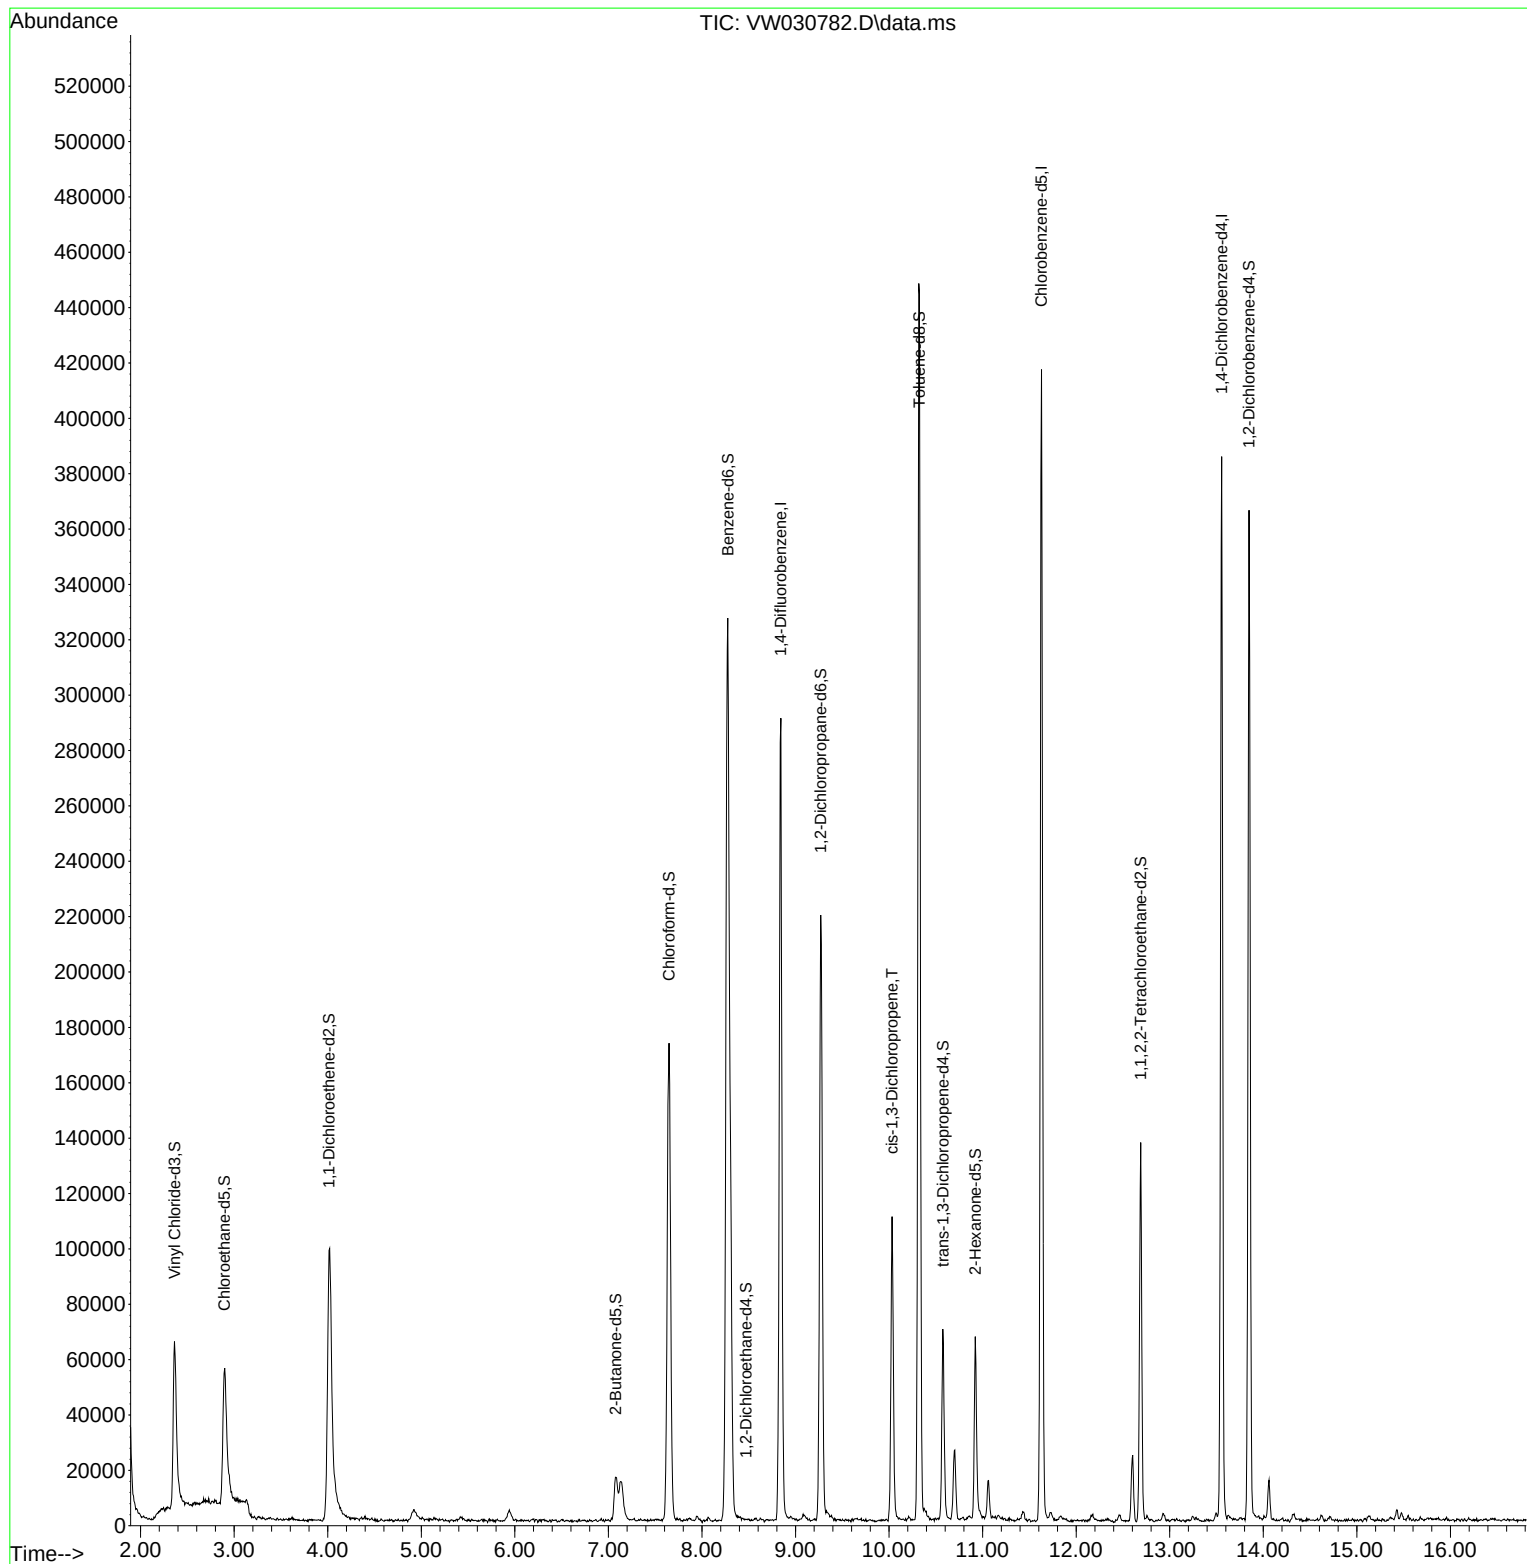

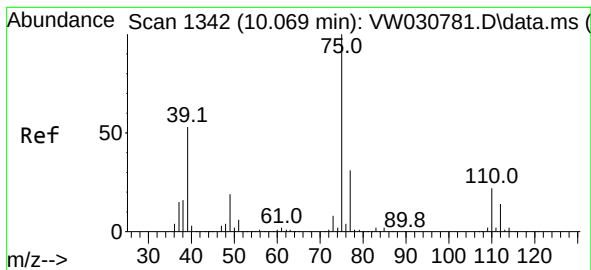

#39
 cis-1,3-Dichloropropene
 Concen: 0.692 ug/L
 RT: 10.032 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW030782.D
 Acq: 28 Oct 2024 13:15

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 3559
 Ion Ratio Lower Upper
 75 100
 77 59.9 21.1 39.1#

