




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102824\
Data File : VW030786.D
Acq On : 28 Oct 2024 15:16
Operator : SY/MD
Sample : P4492-17
Misc : 5.83g/10mL/MSVOA_W/SOIL/A
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4EZ8

Manual IntegrationsAPPROVED

Quant Time: Oct 29 01:34:07 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Oct 29 01:29:12 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 10/29/2024
Supervised By :Mahesh Dadoda 10/29/2024

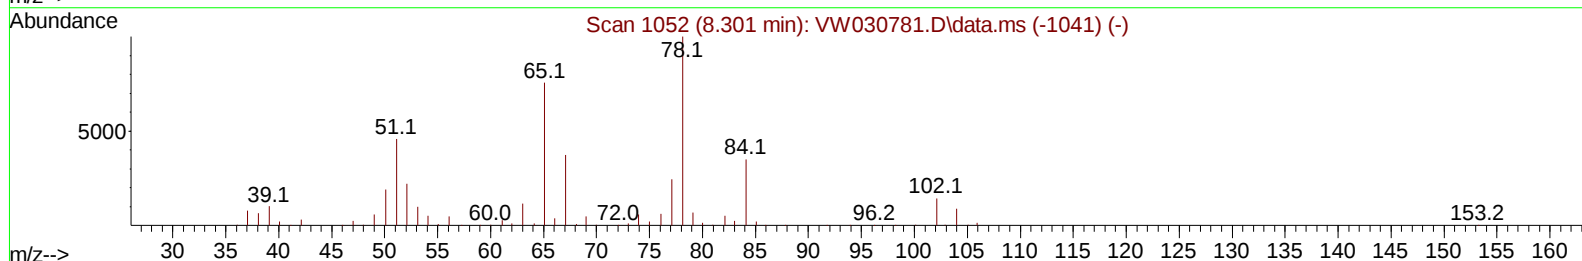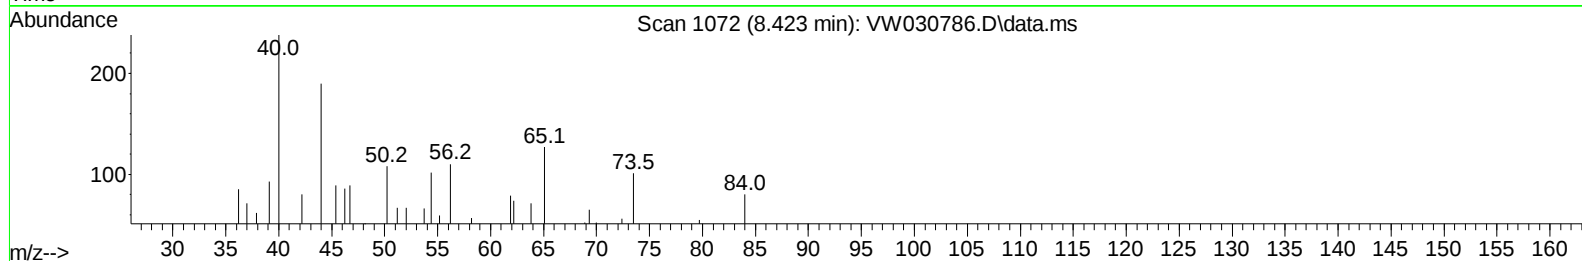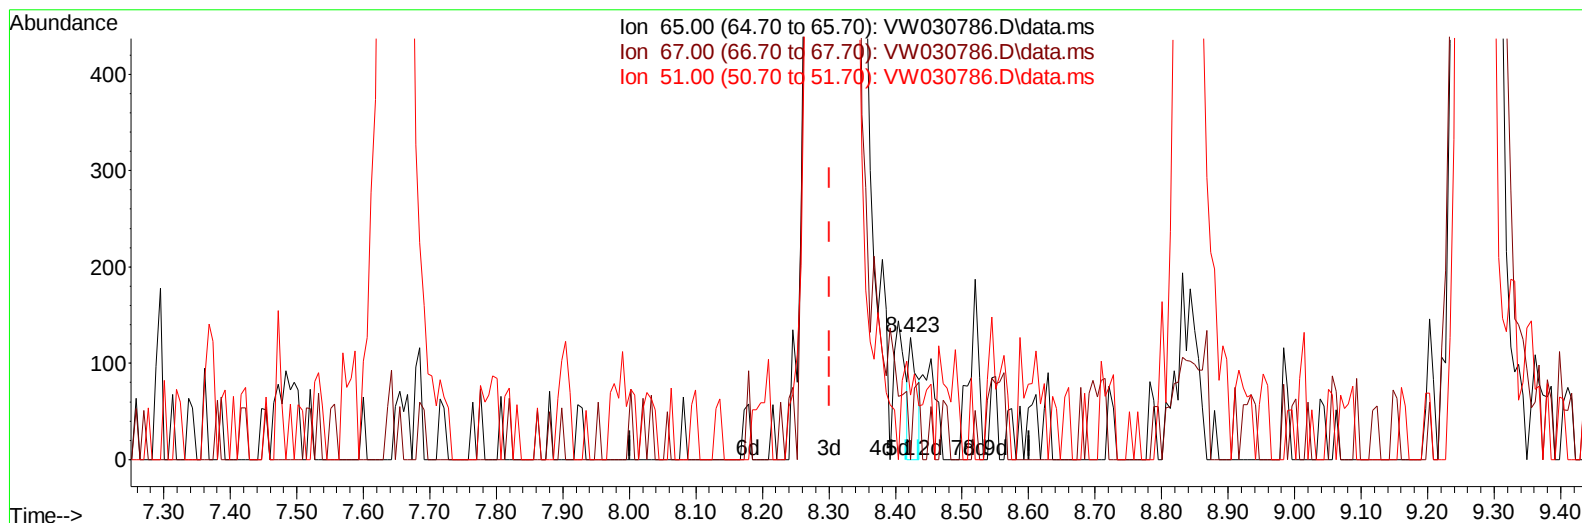

TIC: VW030786.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.423min (+ 0.122) 0.05 ug/L

response 110

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.90	45.45
51.00	109.40	131.82
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102824\
Data File : VW030786.D
Acq On : 28 Oct 2024 15:16
Operator : SY/MD
Sample : P4492-17
Misc : 5.83g/10mL/MSVOA_W/SOIL/A
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4EZ8

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 10/29/2024
Supervised By :Mahesh Dadoda 10/29/2024

Quant Time: Oct 29 01:34:07 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Oct 29 01:29:12 2024
Response via : Initial Calibration

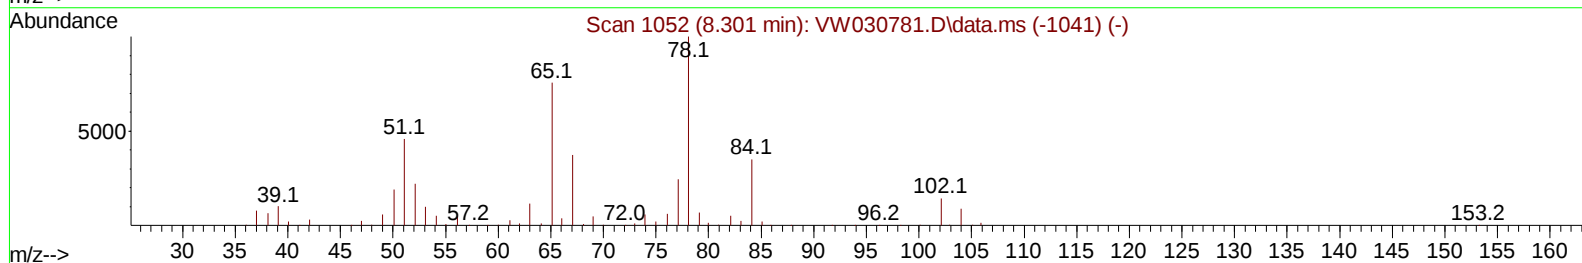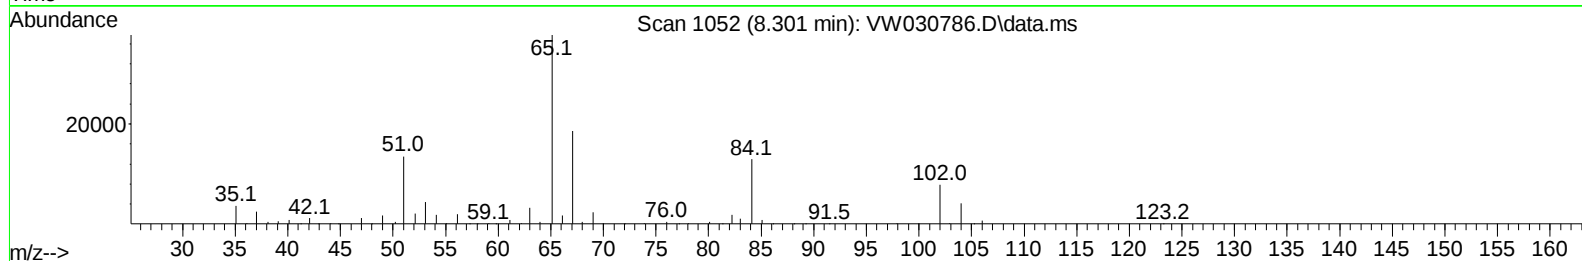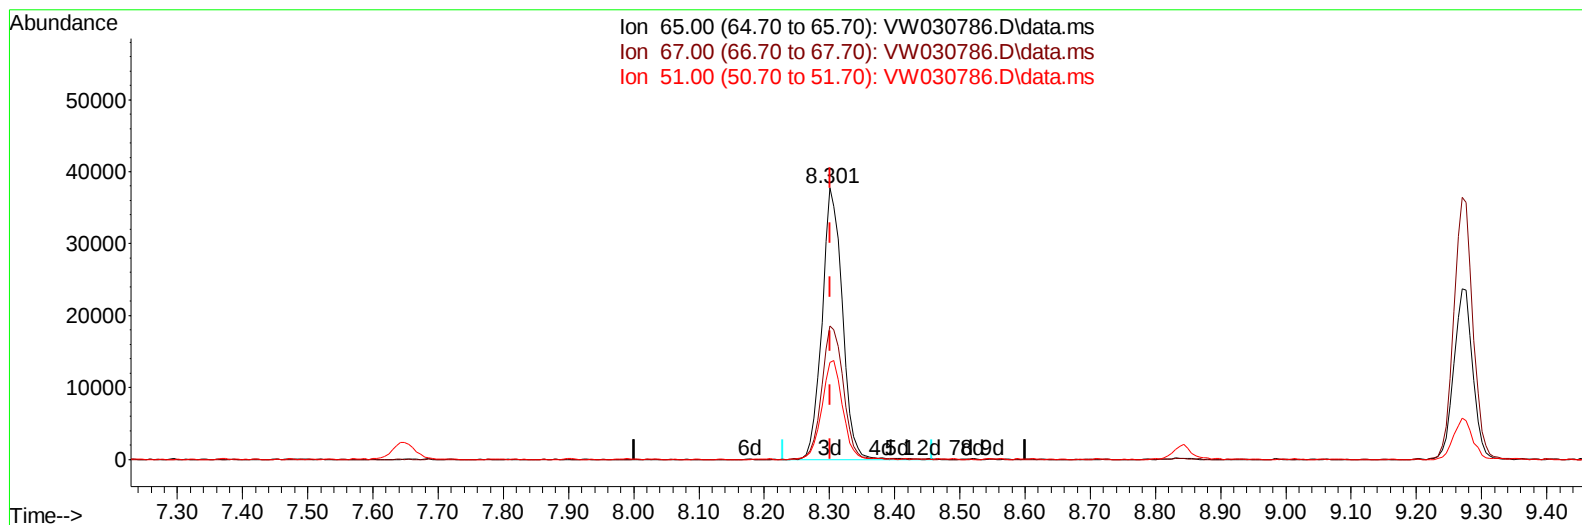

TIC: VW030786.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.301min (-0.000) 35.50 ug/L m

response 81587

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.90	0.06#
51.00	109.40	0.18#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw102824\
 Data File : VW030786.D
 Acq On : 28 Oct 2024 15:16
 Operator : SY/MD
 Sample : P4492-17
 Misc : 5.83g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4EZ8

Manual IntegrationsAPPROVED

Quant Time: Oct 29 01:34:07 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Oct 29 01:29:12 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 10/29/2024
 Supervised By :Mahesh Dadoda 10/29/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.837	114		154539	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		124711	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		42172	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		33890	13.952	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	55.800%		
7) Chloroethane-d5	2.899	69		44495	24.199	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	96.800%		
11) 1,1-Dichloroethene-d2	4.021	65		9993	9.891	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	39.560%#		
21) 2-Butanone-d5	7.075	46		28564	65.341	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	130.680%		
24) Chloroform-d	7.648	84		133249	30.150	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	120.600%		
26) 1,2-Dichloroethane-d4	8.301	65		81587m	35.501	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	142.000%#		
32) Benzene-d6	8.276	84		150107	20.738	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	82.960%		
36) 1,2-Dichloropropane-d6	9.270	67		74031	34.847	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	139.400%#		
41) Toluene-d8	10.325	98		79819	12.080	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	48.320%		
43) trans-1,3-Dichloroprop...	10.581	79		19098	21.468	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	85.880%		
47) 2-Hexanone-d5	10.922	63		19015	69.491	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	138.980%#		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		75936	48.670	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	194.680%#		
66) 1,2-Dichlorobenzene-d4	13.848	152		35111	24.606	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	98.440%		
Target Compounds							
13) Acetone	4.137	43		2428	3.794	ug/L	Qvalue 82

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102824\
Data File : VW030786.D
Acq On : 28 Oct 2024 15:16
Operator : SY/MD
Sample : P4492-17
Misc : 5.83g/10mL/MSVOA_W/SOIL/A
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4EZ8

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 10/29/2024
Supervised By :Mahesh Dadoda 10/29/2024

Quant Time: Oct 29 01:34:07 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Oct 29 01:29:12 2024
Response via : Initial Calibration

