

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102824\
 Data File : VW030786.D
 Acq On : 28 Oct 2024 15:16
 Operator : SY/MD
 Sample : P4492-17
 Misc : 5.83g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4EZ8

Manual Integrations
 APPROVED

Reviewed By :Romaben Patel 10/29/2024
 Supervised By :Mahesh Dadoda 10/29/2024

Quant Time: Oct 29 01:34:07 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Oct 29 01:29:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	154539	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	124711	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	42172	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	33890	13.952	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	55.800%		
7) Chloroethane-d5	2.899	69	44495	24.199	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	96.800%		
11) 1,1-Dichloroethene-d2	4.021	65	9993	9.891	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	39.560%#		
21) 2-Butanone-d5	7.075	46	28564	65.341	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	130.680%		
24) Chloroform-d	7.648	84	133249	30.150	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	120.600%		
26) 1,2-Dichloroethane-d4	8.301	65	81587m	35.501	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	142.000%#		
32) Benzene-d6	8.276	84	150107	20.738	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	82.960%		
36) 1,2-Dichloropropane-d6	9.270	67	74031	34.847	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	139.400%#		
41) Toluene-d8	10.325	98	79819	12.080	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	48.320%		
43) trans-1,3-Dichloroprop...	10.581	79	19098	21.468	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	85.880%		
47) 2-Hexanone-d5	10.922	63	19015	69.491	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	138.980%#		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	75936	48.670	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	194.680%#		
66) 1,2-Dichlorobenzene-d4	13.848	152	35111	24.606	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	98.440%		
Target Compounds					Qvalue	
13) Acetone	4.137	43	2428	3.794	ug/L	82

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102824\
Data File : VW030786.D
Acq On : 28 Oct 2024 15:16
Operator : SY/MD
Sample : P4492-17
Misc : 5.83g/10mL/MSVOA_W/SOIL/A
ALS Vial : 8 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
A4EZ8

Manual Integrations
APPROVED

Reviewed By :Romaben Patel 10/29/2024
Supervised By :Mahesh Dadoda 10/29/2024


Quant Time: Oct 29 01:34:07 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Oct 29 01:29:12 2024
Response via : Initial Calibration

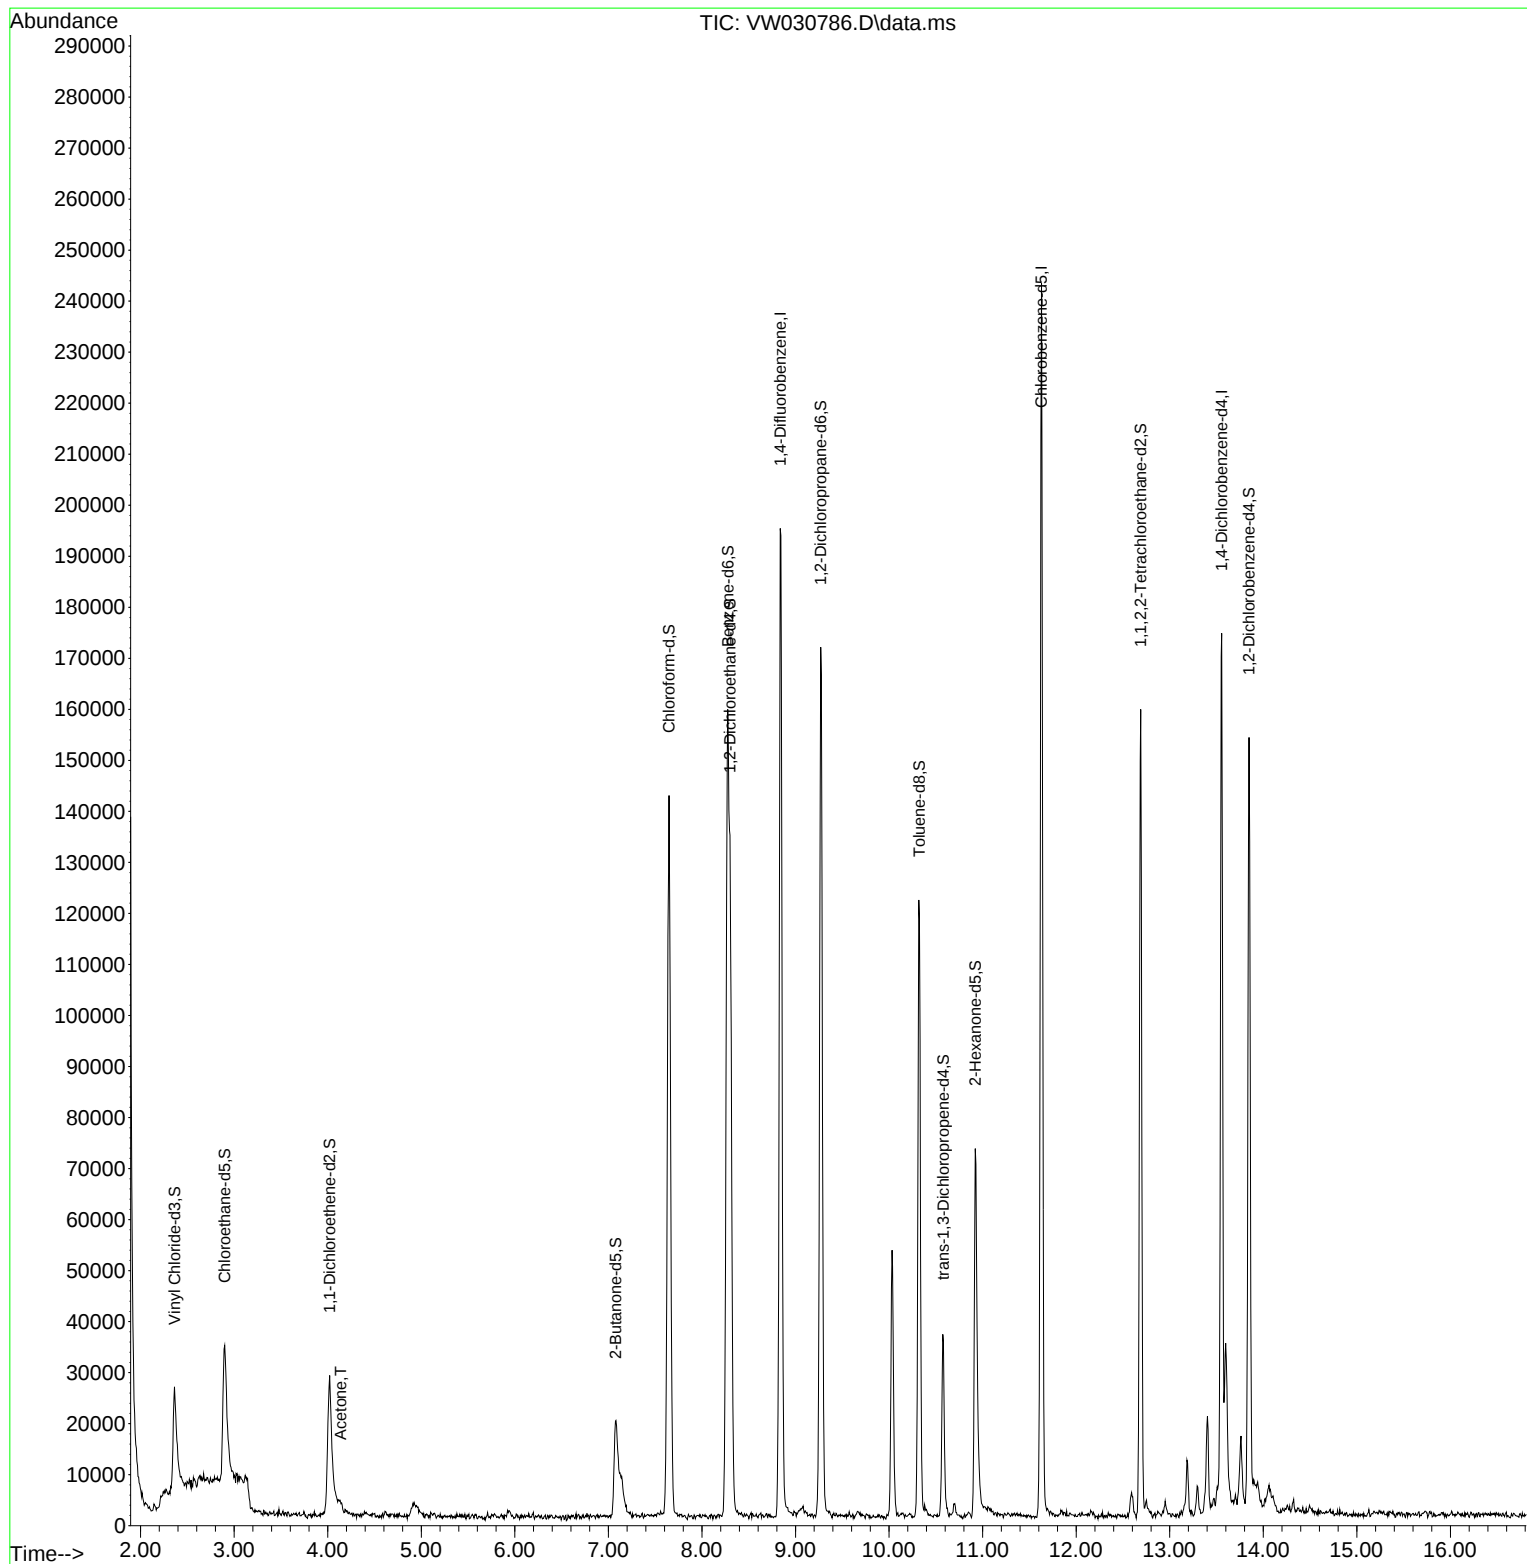

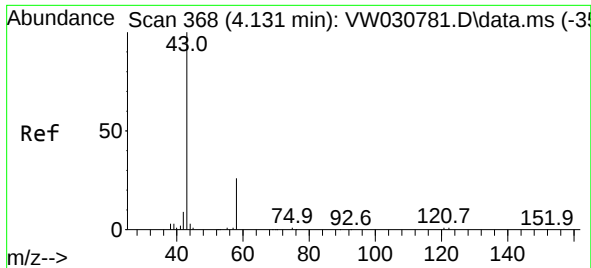

#13
Acetone
Concen: 3.794 ug/L
RT: 4.137 min Scan# 30
Delta R.T. 0.006 min
Lab File: VW030786.D
Acq: 28 Oct 2024 15:16

Instrument :
MSVOA_W
ClientSampleId :
A4EZ8

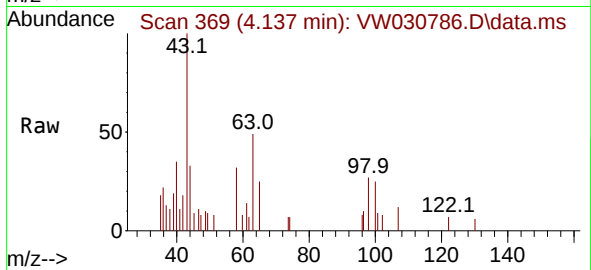

Tgt Ion: 43 Resp: 2428
Ion Ratio Lower Upper
43 100
58 19.4 0.0 57.6

Manual Integrations
APPROVED

Reviewed By :Romaben Patel 10/29/2024
Supervised By :Mahesh Dadoda 10/29/2024

