
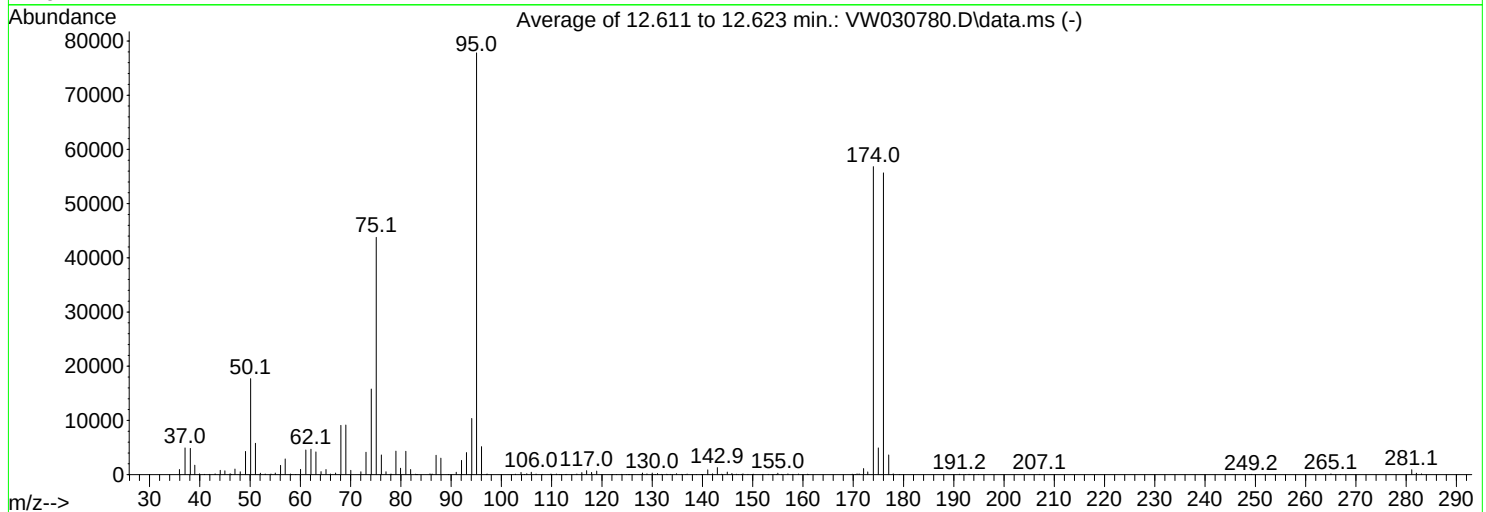


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102824\
Data File : VW030780.D
Acq On : 28 Oct 2024 09:40
Operator : SY/MD
Sample : BFB585
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB585

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Title : SFAM01.0
Last Update : Tue Oct 29 01:29:12 2024

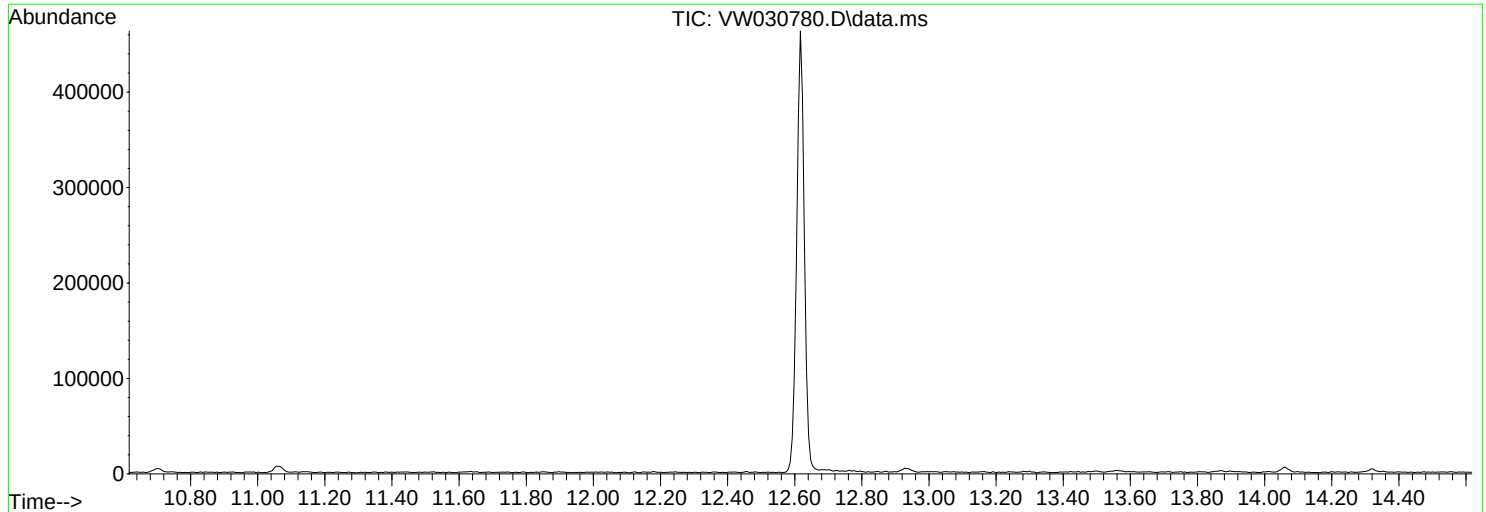

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.8	17723	PASS
75	95	30	80	56.3	43784	PASS
95	95	100	100	100.0	77813	PASS
96	95	5	9	6.6	5155	PASS
173	174	0.00	2	0.9	492	PASS
174	95	50	120	73.0	56808	PASS
175	174	5	9	8.7	4945	PASS
176	174	95	101	98.0	55656	PASS
177	176	5	9	6.5	3637	PASS

m/z	Abundance
35.40	76.0
35.90	84.0
37.10	78.0
38.10	64.0
38.90	110.0
40.00	198.0
41.20	56.0
42.20	96.0
44.00	147.0
45.00	52.0
46.60	55.0
47.60	61.0
48.20	73.0
50.30	60.0
52.10	64.0
52.90	52.0
57.00	100.0
66.40	55.0
73.30	59.0
99.70	55.0

Instrument :
MSVOA_W
ClientSampleId :
BFB585

m/z	Abundance
36.00	1273.0
37.00	4848.0
38.10	4806.0
39.00	1776.0
39.90	414.0
40.90	149.0
41.80	65.0
42.20	77.0
43.10	86.0
44.20	914.0
45.10	808.0
46.10	221.0
47.00	1016.0
48.10	650.0
49.10	4066.0
50.10	16704.0
51.10	5606.0
52.00	294.0
53.20	184.0
54.10	137.0
54.90	273.0
56.00	1726.0
57.00	2705.0
58.00	113.0
59.10	66.0
60.10	1176.0
61.10	4589.0
62.10	4644.0
63.10	3997.0
64.20	516.0
65.10	1129.0
66.00	152.0
67.00	285.0
68.00	8103.0
69.00	8696.0
70.00	651.0
72.00	460.0
73.10	4021.0
74.10	14661.0
75.10	39688.0
76.10	3545.0
77.00	531.0
77.90	301.0
79.00	4300.0
80.00	960.0
81.00	3849.0
81.90	860.0
83.00	157.0
86.20	229.0
87.00	3335.0
87.90	2974.0
91.00	386.0
92.10	2515.0
93.00	3737.0
94.10	9540.0
95.10	68496.0
96.10	4828.0
97.00	203.0
102.70	79.0
103.90	386.0
104.60	102.0
105.00	81.0
106.00	368.0
106.80	112.0
108.10	60.0
109.80	102.0
111.00	104.0
112.00	60.0
112.80	106.0
114.90	135.0
116.10	271.0
117.00	752.0
117.90	446.0
118.90	691.0
122.90	56.0
123.90	96.0
125.30	132.0
127.80	198.0
128.10	224.0
129.00	144.0
130.00	266.0
130.60	76.0
131.10	156.0
132.90	135.0
133.70	113.0
134.80	71.0
137.00	153.0
141.00	689.0
142.00	189.0
143.00	1364.0
143.90	79.0
145.00	581.0

Instrument :
MSVOA_W
ClientSampleId :
BFB585

145.90	206.0
146.80	85.0
148.10	198.0
149.00	102.0
152.00	74.0
153.00	65.0
153.90	72.0
154.70	198.0
155.10	214.0
155.80	65.0
157.00	165.0
159.20	90.0
160.90	111.0
169.80	68.0
170.80	310.0
172.10	1078.0
174.00	49968.0
175.00	3960.0
176.00	45488.0
177.00	2696.0
178.10	139.0
179.20	76.0
191.20	185.0
192.30	62.0
193.00	153.0
194.10	61.0
194.90	67.0
207.10	185.0
248.80	123.0
249.20	150.0
265.10	165.0
266.90	99.0
281.10	1304.0
282.10	376.0
283.10	249.0

Instrument :
MSVOA_W
ClientSampleId :
BFB585

m/z	Abundance
36.00	1063.0
37.10	5919.0
38.10	5654.0
39.10	2086.0
40.00	360.0
41.90	103.0
42.30	94.0
43.00	180.0
44.00	1078.0
45.00	816.0
46.00	228.0
46.30	217.0
47.10	1074.0
48.00	686.0
49.10	4945.0
50.10	20480.0
51.10	6696.0
52.00	399.0
53.00	207.0
54.20	93.0
55.00	419.0
56.10	1836.0
57.10	3381.0
58.10	232.0
60.00	920.0
61.10	4971.0
62.10	5254.0
63.10	4738.0
64.10	617.0
65.10	1078.0
66.00	192.0
67.00	397.0
68.10	10630.0
69.10	10120.0
70.10	810.0
72.00	612.0
73.10	4766.0
74.10	16936.0
75.10	49272.0
76.10	3923.0
77.10	560.0
79.00	4972.0
80.00	1440.0
81.00	4976.0
82.00	1080.0
82.90	92.0
83.30	82.0
85.90	234.0
87.00	4230.0
88.00	3201.0
91.00	471.0
92.00	2718.0
93.00	4669.0
94.10	12080.0
95.10	89360.0
96.10	5730.0
97.20	233.0
102.80	68.0
103.90	354.0
105.10	222.0
105.90	435.0
106.90	130.0
108.10	143.0
109.90	109.0
111.00	123.0
111.80	69.0
113.00	101.0
115.00	145.0
116.00	449.0
117.00	823.0
118.00	426.0
118.90	654.0
122.10	57.0
124.00	74.0
124.90	59.0
125.50	69.0
128.10	398.0
129.00	191.0
130.10	375.0
131.00	243.0
131.80	60.0
132.90	96.0
133.50	104.0
134.80	195.0
135.90	81.0
136.90	172.0
139.80	104.0
141.00	1028.0
142.00	138.0
143.00	1249.0
143.80	98.0
144.90	513.0

Instrument :
MSVOA_W
ClientSampleId :
BFB585

145.80	242.0
146.70	126.0
148.00	244.0
149.10	123.0
150.10	100.0
152.10	76.0
153.10	76.0
153.80	67.0
154.20	67.0
154.90	275.0
155.70	78.0
157.10	140.0
158.00	84.0
159.00	161.0
161.10	136.0
169.80	86.0
170.60	145.0
171.10	215.0
172.00	1119.0
172.90	1475.0
174.00	67648.0
175.00	5731.0
176.00	60280.0
177.10	4121.0
177.90	100.0
191.10	126.0
193.20	144.0
265.00	165.0
281.10	1094.0
282.00	254.0
283.10	145.0

Instrument :
MSVOA_W
ClientSampleId :
BFB585

m/z	Abundance
36.10	713.0
37.00	4289.0
38.10	4258.0
39.10	1727.0
40.00	265.0
40.90	77.0
42.10	96.0
43.00	158.0
44.10	864.0
45.10	698.0
46.00	127.0
46.90	1041.0
48.00	525.0
49.10	3865.0
50.10	16166.0
51.00	5024.0
52.10	308.0
53.00	166.0
54.10	106.0
55.10	202.0
56.10	1540.0
57.00	2926.0
58.30	124.0
59.10	75.0
60.00	806.0
61.10	4122.0
62.10	4218.0
63.10	3842.0
64.00	532.0
65.00	621.0
66.20	158.0
67.00	230.0
68.10	8520.0
69.10	8635.0
70.10	908.0
72.10	562.0
73.00	3819.0
74.10	15807.0
75.10	42392.0
76.10	3461.0
77.10	480.0
78.10	297.0
79.00	3749.0
79.90	1103.0
81.00	4065.0
82.00	901.0
83.10	142.0
85.70	199.0
86.20	168.0
87.00	3147.0
88.00	2967.0
89.50	53.0
91.00	460.0
92.00	2686.0
93.10	3864.0
94.10	9445.0
95.00	75584.0
96.00	4906.0
97.10	129.0
102.90	115.0
103.90	506.0
105.00	204.0
105.90	497.0
107.00	125.0
109.80	134.0
110.90	156.0
111.60	77.0
113.00	76.0
115.10	84.0
115.90	432.0
116.80	625.0
117.90	386.0
119.00	639.0
122.10	59.0
126.00	61.0
128.00	297.0
128.90	139.0
129.90	288.0
131.00	225.0
131.80	93.0
133.10	58.0
134.90	266.0
135.90	73.0
136.70	135.0
138.80	69.0
140.10	131.0
141.10	917.0
142.00	159.0
142.90	1320.0
143.90	61.0
145.00	321.0
145.90	195.0

Instrument :
MSVOA_W
ClientSampleId :
BFB585

146.70	69.0
147.10	72.0
147.80	192.0
150.10	161.0
153.20	59.0
155.00	266.0
155.80	75.0
156.90	178.0
158.00	113.0
159.20	146.0
160.90	134.0
169.80	95.0
170.40	85.0
171.20	260.0
172.00	1174.0
174.00	52808.0
175.00	5144.0
176.00	61200.0
177.00	4095.0
177.90	211.0
193.00	53.0
265.10	136.0
281.00	371.0
282.00	137.0
282.90	83.0

Instrument :
MSVOA_W
ClientSampleId :
BFB585