

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW103018\
 Data File : VW006450.D
 Acq On : 29 Oct 2018 12:57
 Operator : SY/AP
 Sample : J5705-01
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A40B3

Quant Time: Oct 30 05:11:11 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100918S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 30 04:53:39 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	376295	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	352964	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	186434	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	111939	26.38	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	105.52%
7) Chloroethane-d5	2.90	69	97537	26.70	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	106.80%
10) 1,1-Dichloroethene-d2	4.01	63	153737	18.86	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	75.44%
20) 2-Butanone-d5	7.09	46	57462	40.85	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	81.70%
24) Chloroform-d	7.65	84	205357	25.19	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	100.76%
26) 1,2-Dichloroethane-d4	8.31	65	117404	26.03	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	104.12%
29) Benzene-d6	8.27	84	417840	26.07	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	104.28%
33) 1,2-Dichloropropane-d6	9.27	67	119435	24.70	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	98.80%
37) Toluene-d8	10.33	98	413134	25.78	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	103.12%
38) trans-1,3-Dichloropropene-	10.58	79	54973	23.39	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	93.56%
39) 2-Hexanone-d5	10.93	63	47644	40.77	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	81.54%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	111418	23.69	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.76%
61) 1,2-Dichlorobenzene-d4	13.86	152	171119	26.78	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	107.12%


Target Compounds					Ovalue
13) Acetone	4.15	43	41368	29.110 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW103018\
Data File : VW006450.D
Acq On : 29 Oct 2018 12:57
Operator : SY/AP
Sample : J5705-01
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A40B3

Quant Time: Oct 30 05:11:11 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100918S.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 30 04:53:39 2018
Response via : Initial Calibration

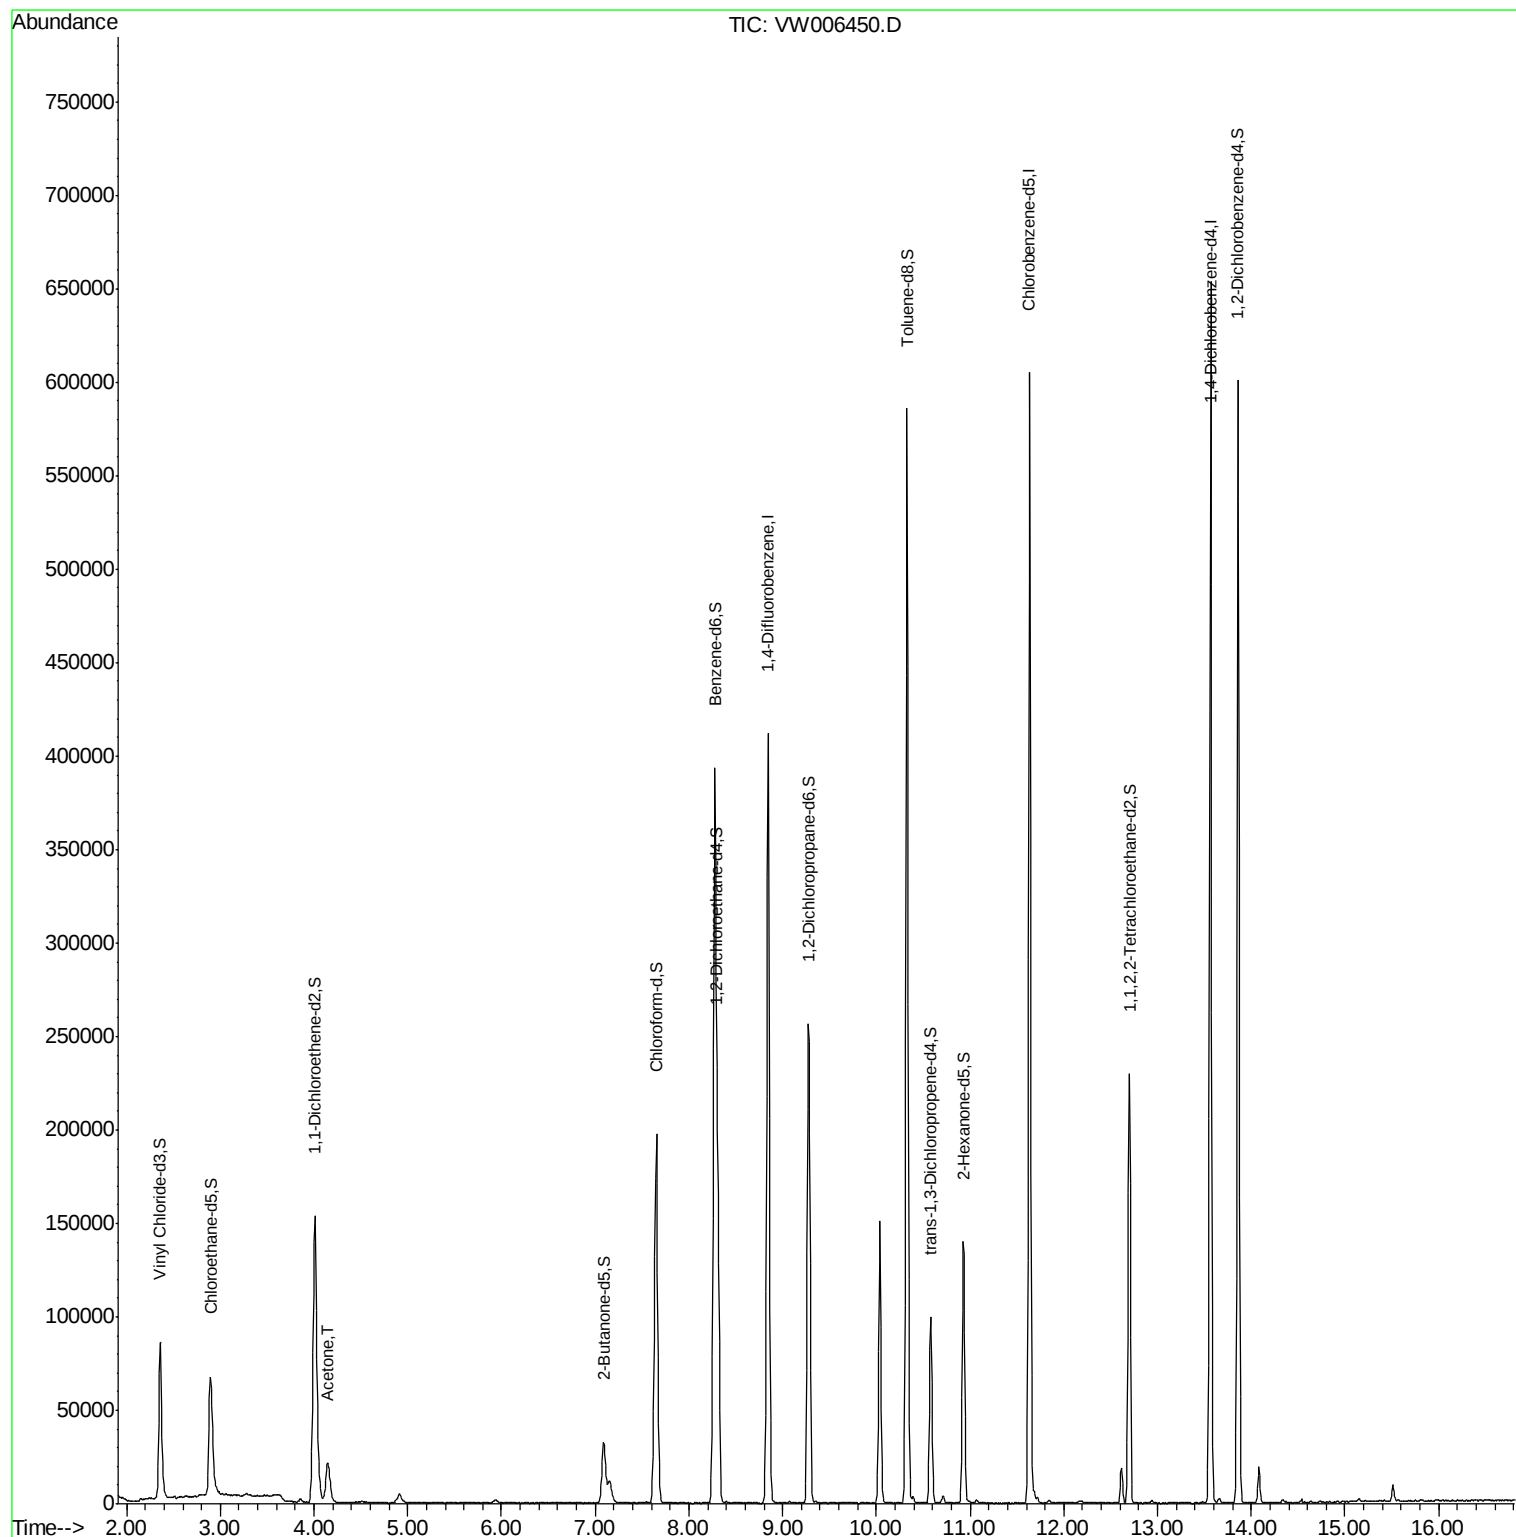

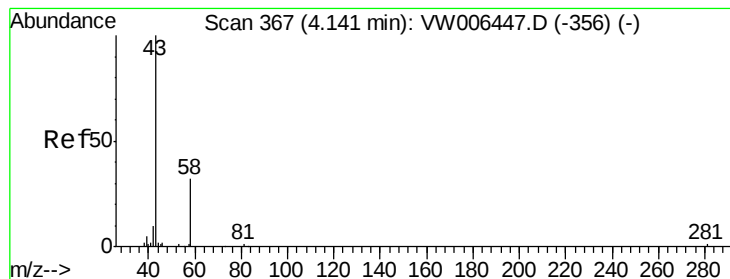

#13

Acetone

Concen: 29.110 ug/L

RT: 4.15 min Scan# 368

Delta R.T. 0.01 min

Lab File: VW006450.D

Acq: 29 Oct 2018 12:57

Instrument :

MSVOA_W

ClientSampleId :

A40B3

Tot Ion: 43 Resp: 41368

Ion Ratio Lower Upper

43 100

58 30.3 0.0 61.2

