

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW103018\
 Data File : VW006463.D
 Acq On : 29 Oct 2018 18:33
 Operator : SY/AP
 Sample : J5705-12
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK01

Quant Time: Oct 30 06:38:51 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100918S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 30 04:53:39 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	308272	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	293900	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	154387	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	101223	29.12	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	116.48%
7) Chloroethane-d5	2.90	69	86148	28.79	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	115.16%
10) 1,1-Dichloroethene-d2	4.01	63	139217	20.85	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	83.40%
20) 2-Butanone-d5	7.08	46	65094	56.49	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	112.98%
24) Chloroform-d	7.65	84	186322	27.90	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	111.60%
26) 1,2-Dichloroethane-d4	8.31	65	108966	29.50	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	118.00%
29) Benzene-d6	8.28	84	384070	28.78	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	115.12%
33) 1,2-Dichloropropane-d6	9.28	67	109000	27.07	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	108.28%
37) Toluene-d8	10.33	98	376490	28.21	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	112.84%
38) trans-1,3-Dichloropropene-	10.58	79	48058	24.56	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	98.24%
39) 2-Hexanone-d5	10.93	63	52115	53.56	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	107.12%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	110661	28.26	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	113.04%
61) 1,2-Dichlorobenzene-d4	13.86	152	157697	29.80	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	119.20%


Target Compounds					Ovalue
13) Acetone	4.12	43	2990	2.568 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW103018\
Data File : VW006463.D
Acq On : 29 Oct 2018 18:33
Operator : SY/AP
Sample : J5705-12
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK01

Quant Time: Oct 30 06:38:51 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100918S.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 30 04:53:39 2018
Response via : Initial Calibration

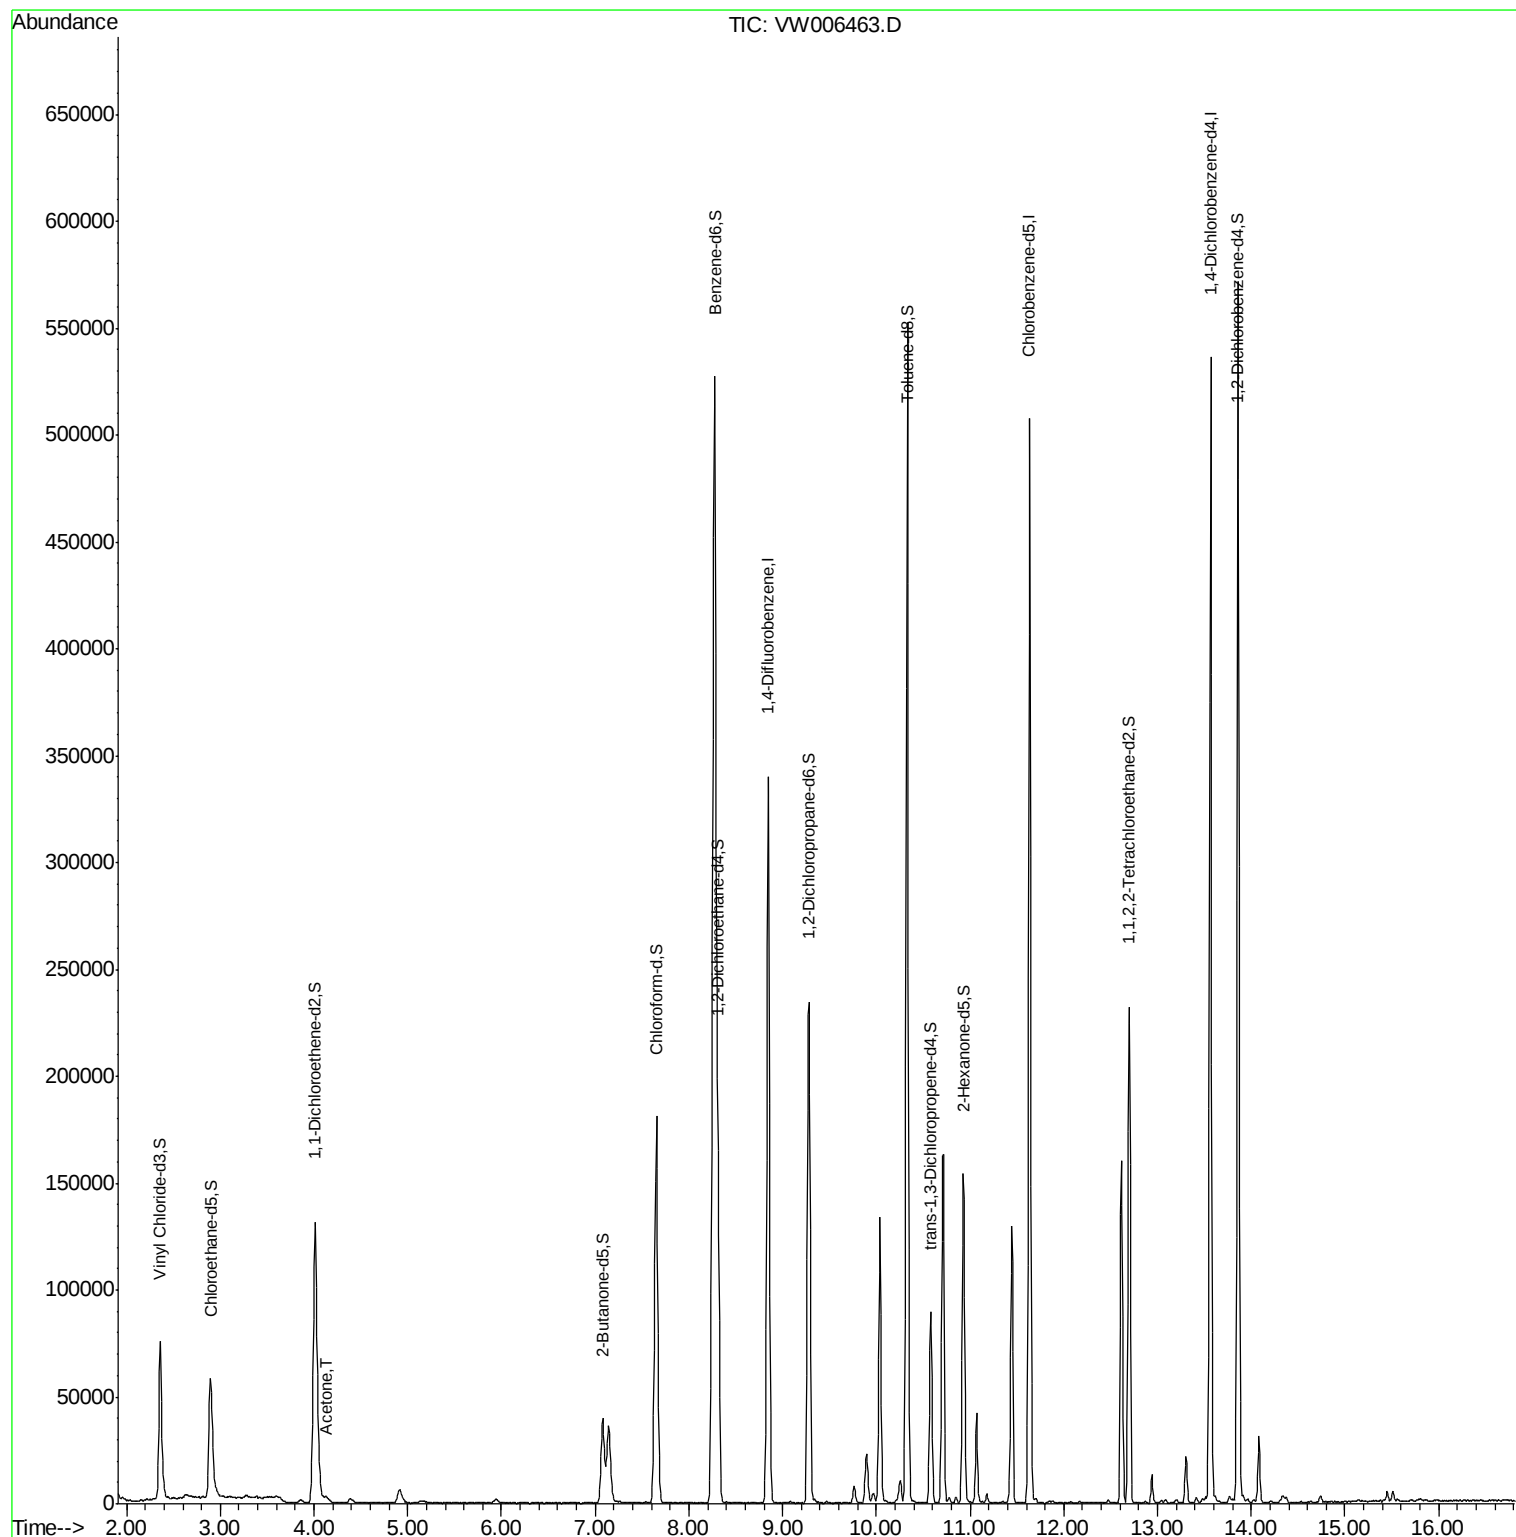

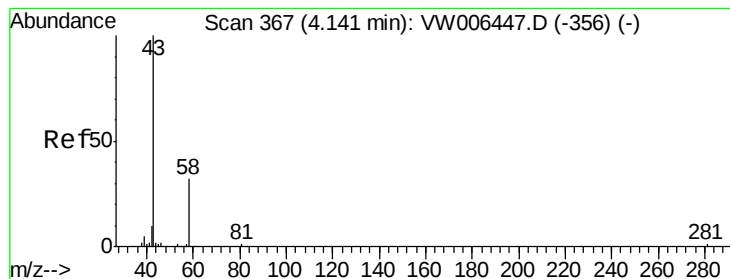

#13
 Acetone
 Concen: 2.568 ug/L
 RT: 4.12 min Scan# 364
 Delta R.T. -0.02 min
 Lab File: VW006463.D
 Acq: 29 Oct 2018 18:33

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK01

Tot Ion: 43 Resp: 2990
 Ion Ratio Lower Upper
 43 100
 58 29.8 0.0 61.2

