


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW103018\
 Data File : VW006446.D
 Acq On : 29 Oct 2018 09:29
 Operator : SY/AP
 Sample : BFB95
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB95

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100918S.M
 Title : VOC Analysis
 Last Update : Tue Oct 30 04:53:39 2018

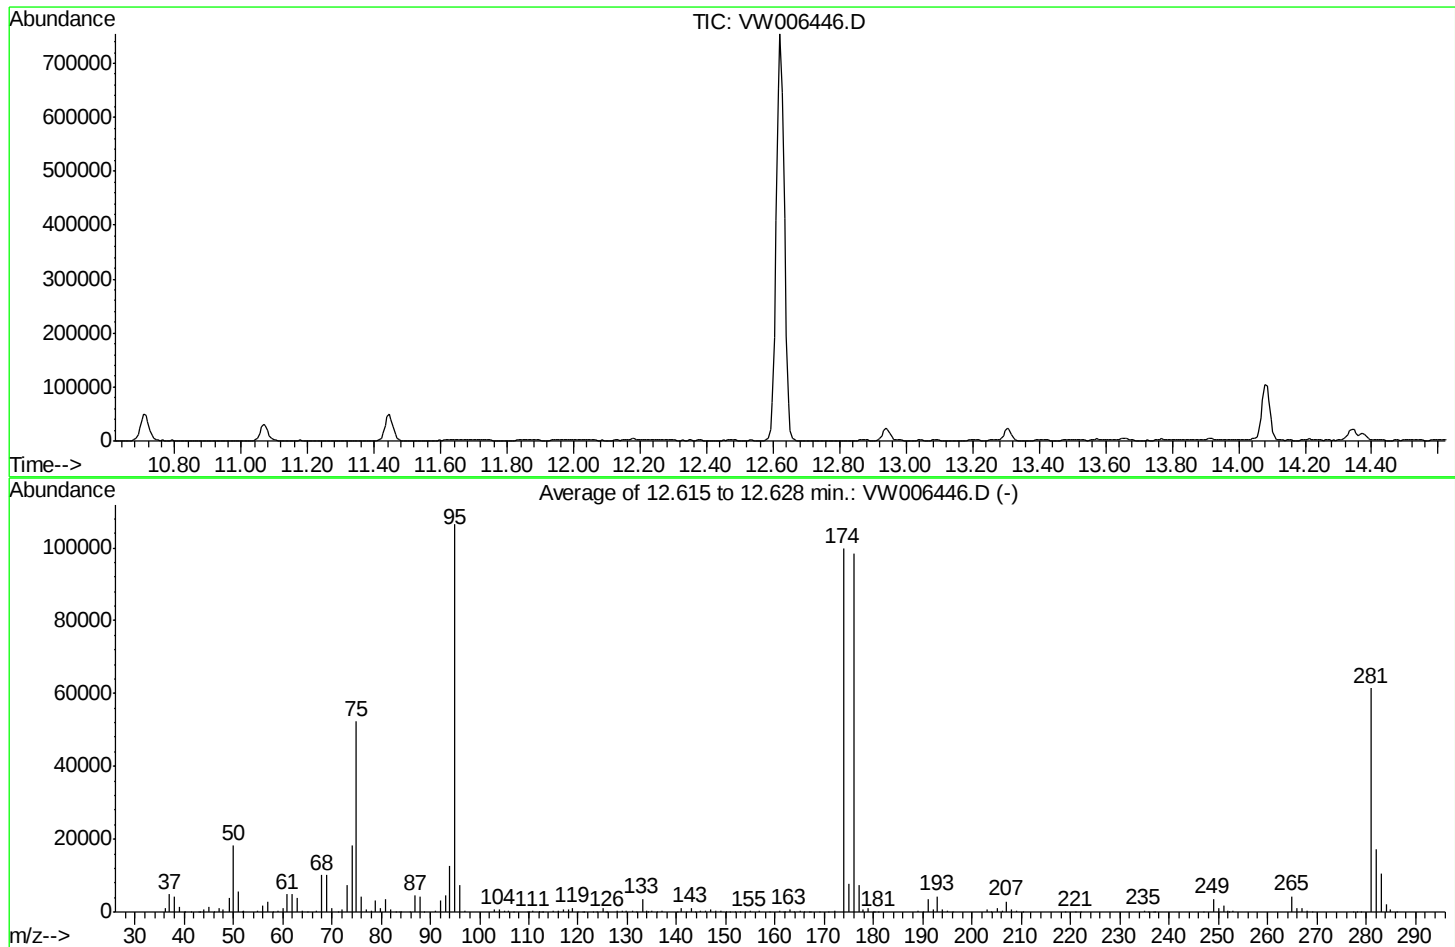

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	18213	PASS
75	95	30	80	49.2	52360	PASS
95	95	100	100	100.0	106442	PASS
96	95	5	9	7.1	7521	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	93.7	99784	PASS
175	174	5	9	7.8	7761	PASS
176	174	95	101	98.5	98282	PASS
177	176	5	9	7.6	7438	PASS

Scan 1750 (12.573 min): VW006446.D
BFB95

m/z	Abundance
39.00	78.0
39.90	95.0
41.10	119.0
43.90	194.0
68.90	57.0
73.10	54.0
169.10	97.0
206.90	147.0
208.10	60.0
280.90	54.0

Instrument :
MSVOA_W
ClientSampleId :
BFB95

m/z	Abundance
36.00	884.0
37.00	4560.0
38.00	4119.0
39.00	1606.0
40.00	121.0
41.10	122.0
43.00	242.0
44.00	793.0
45.00	1459.0
46.10	176.0
47.00	835.0
48.00	608.0
49.00	4045.0
50.00	16960.0
51.00	5421.0
52.20	300.0
55.00	312.0
56.00	1591.0
57.00	2468.0
58.10	156.0
59.00	604.0
60.00	1024.0
61.00	4745.0
62.00	4726.0
63.00	3442.0
64.00	321.0
65.10	151.0
67.00	255.0
68.00	9462.0
69.00	9802.0
70.10	841.0
71.20	105.0
71.90	549.0
73.10	7937.0
74.00	16536.0
75.00	48880.0
76.00	4172.0
77.00	573.0
77.90	461.0
78.90	3165.0
79.90	993.0
80.90	3270.0
81.90	724.0
83.10	131.0
83.70	73.0
85.90	104.0
87.00	4123.0
88.00	4200.0
88.80	363.0
91.00	384.0
92.00	2758.0
93.00	4166.0
94.00	11012.0
95.00	94648.0
96.00	6846.0
97.00	261.0
102.90	783.0
103.90	751.0
105.00	349.0
105.90	519.0
106.90	125.0
110.10	306.0
110.80	432.0
112.20	260.0
113.00	111.0
115.00	426.0
115.80	391.0
116.90	750.0
117.90	862.0
119.00	1292.0
120.00	159.0
120.90	184.0
125.00	1339.0
125.70	382.0
128.00	405.0
128.90	247.0
129.80	335.0
130.90	252.0
131.90	133.0
133.00	4701.0
133.80	1077.0
134.90	579.0
136.10	84.0
137.00	101.0
140.90	909.0
142.00	93.0
142.90	1022.0
144.00	84.0
145.00	170.0
145.80	191.0
146.90	583.0
147.80	365.0

Instrument :
MSVOA_W
ClientSampleId :
BFB95

149.00	393.0
149.90	172.0
150.80	53.0
153.00	71.0
153.90	103.0
154.80	182.0
156.90	172.0
158.90	186.0
160.80	399.0
162.00	130.0
162.90	762.0
163.90	146.0
165.00	677.0
165.80	119.0
166.80	151.0
169.00	118.0
170.90	51.0
172.10	272.0
173.90	81624.0
174.90	6371.0
175.90	81312.0
177.00	6772.0
177.90	692.0
179.00	1168.0
179.90	294.0
181.00	172.0
189.00	473.0
189.90	233.0
191.00	4564.0
192.10	1092.0
193.00	5752.0
194.00	1065.0
195.00	666.0
195.90	98.0
203.00	753.0
204.00	128.0
205.00	1300.0
206.10	340.0
207.10	3991.0
208.00	913.0
209.00	525.0
210.20	61.0
219.00	136.0
221.00	255.0
221.90	62.0
235.00	569.0
235.90	237.0
236.90	209.0
246.90	122.0
249.00	4250.0
250.00	1037.0
251.00	2103.0
251.90	382.0
253.00	354.0
265.00	5284.0
266.00	1445.0
267.00	1256.0
267.90	329.0
269.00	156.0
277.50	55.0
279.00	213.0
281.10	72592.0
282.00	20744.0
283.00	12916.0
284.00	2622.0
285.00	807.0
286.10	120.0

Instrument :
MSVOA_W
ClientSampleId :
BFB95

m/z	Abundance
36.10	1015.0
37.00	5169.0
38.00	4587.0
39.00	1779.0
40.00	220.0
40.90	64.0
41.30	100.0
43.00	190.0
44.00	907.0
45.00	1363.0
46.00	151.0
47.10	1149.0
48.00	622.0
49.10	4259.0
50.00	20424.0
51.00	6110.0
52.10	280.0
55.00	337.0
56.00	1758.0
57.00	3339.0
57.90	168.0
59.00	470.0
60.00	1158.0
61.00	5377.0
62.00	5344.0
63.00	4116.0
64.00	397.0
65.10	178.0
67.00	324.0
68.00	11064.0
69.00	11805.0
70.00	964.0
71.20	61.0
72.00	683.0
73.00	8307.0
74.00	20048.0
75.00	58384.0
76.00	4991.0
77.00	872.0
78.00	505.0
78.90	3547.0
79.90	1162.0
80.90	4049.0
81.90	781.0
83.00	106.0
84.10	106.0
85.80	75.0
87.00	5147.0
88.00	4849.0
90.90	382.0
92.00	3625.0
93.00	4836.0
94.00	14934.0
95.00	118688.0
96.00	8665.0
97.00	244.0
103.00	728.0
103.90	613.0
104.90	338.0
106.00	616.0
107.00	147.0
109.80	286.0
110.90	268.0
111.90	200.0
112.70	160.0
115.00	271.0
115.90	427.0
116.90	1123.0
118.00	959.0
118.90	1139.0
120.00	177.0
120.90	145.0
123.80	62.0
125.00	1287.0
127.80	495.0
128.90	231.0
129.90	419.0
131.00	326.0
131.90	160.0
133.00	4110.0
134.90	563.0
136.00	77.0
137.00	204.0
140.10	124.0
141.00	1060.0
142.00	150.0
142.90	1306.0
143.80	73.0
145.00	192.0
145.80	206.0
146.90	688.0
147.90	426.0

Instrument :
MSVOA_W
ClientSampleId :
BFB95

148.80	269.0
149.90	133.0
152.90	89.0
154.00	51.0
154.90	262.0
156.90	200.0
158.80	120.0
160.90	416.0
161.90	84.0
163.00	686.0
163.90	169.0
165.00	440.0
165.70	68.0
167.10	110.0
169.00	109.0
172.00	497.0
173.90	109960.0
174.90	8561.0
175.90	108120.0
176.90	8072.0
178.00	609.0
179.00	892.0
179.70	134.0
180.10	87.0
189.00	362.0
190.00	122.0
191.00	3494.0
192.00	825.0
193.00	4745.0
194.00	849.0
195.00	497.0
203.00	632.0
203.90	128.0
205.00	798.0
206.10	184.0
207.10	3214.0
208.10	645.0
209.10	338.0
219.00	166.0
221.00	189.0
221.90	61.0
235.00	562.0
235.90	116.0
236.90	152.0
247.00	151.0
249.00	4208.0
250.00	987.0
251.00	1594.0
251.90	334.0
252.90	168.0
265.00	4787.0
266.10	1277.0
267.00	1506.0
268.00	314.0
269.00	109.0
277.40	64.0
278.80	210.0
281.10	67256.0
282.00	18856.0
283.00	11228.0
284.10	2243.0
285.00	749.0
286.10	77.0

Instrument :
MSVOA_W
ClientSampleId :
BFB95

m/z	Abundance
36.00	797.0
37.00	4637.0
38.00	3943.0
39.00	1580.0
40.20	127.0
41.10	80.0
42.90	78.0
43.20	81.0
44.00	755.0
45.00	964.0
46.10	87.0
46.90	889.0
48.00	592.0
49.00	3783.0
50.00	17256.0
51.00	5190.0
51.90	203.0
55.00	381.0
56.00	1491.0
57.00	2675.0
57.90	160.0
59.00	202.0
60.00	834.0
61.00	4524.0
62.00	4400.0
63.00	3866.0
64.00	301.0
65.10	147.0
66.90	258.0
68.00	9848.0
69.00	9643.0
70.00	885.0
72.00	595.0
73.00	6110.0
74.00	17944.0
75.00	49816.0
76.00	4039.0
77.00	606.0
77.90	368.0
78.90	3341.0
80.00	903.0
80.90	3408.0
82.00	689.0
83.10	111.0
86.90	4055.0
87.90	3999.0
90.90	417.0
92.00	3394.0
93.00	4447.0
94.00	12062.0
95.00	105992.0
96.00	7052.0
97.00	206.0
103.00	301.0
103.90	496.0
104.90	244.0
105.80	472.0
106.90	106.0
109.90	195.0
111.00	285.0
112.00	193.0
112.90	123.0
115.10	220.0
115.90	496.0
116.90	748.0
117.90	713.0
119.00	1052.0
120.00	82.0
120.90	55.0
121.20	56.0
123.00	51.0
123.80	81.0
125.00	534.0
125.90	245.0
127.90	458.0
128.90	225.0
129.90	365.0
131.00	189.0
132.00	89.0
133.00	1957.0
134.10	271.0
135.00	447.0
135.90	58.0
136.90	263.0
140.90	1163.0
142.90	1106.0
143.80	82.0
144.80	164.0
145.10	156.0
145.80	245.0
147.00	406.0
147.90	340.0

Instrument :
MSVOA_W
ClientSampleId :
BFB95

149.00	196.0
150.00	191.0
151.90	53.0
152.90	123.0
154.10	52.0
154.80	258.0
156.90	310.0
158.90	195.0
160.90	349.0
161.70	54.0
162.90	449.0
163.90	53.0
164.90	305.0
165.80	76.0
167.00	57.0
168.90	101.0
172.00	447.0
173.90	107768.0
174.90	8353.0
175.90	105416.0
177.00	7471.0
178.00	368.0
179.00	709.0
180.00	120.0
181.00	56.0
188.90	257.0
190.10	82.0
191.00	2381.0
192.00	487.0
193.00	2638.0
194.10	538.0
195.00	242.0
203.00	303.0
205.10	608.0
206.10	175.0
207.00	2114.0
207.90	340.0
209.00	318.0
218.90	59.0
221.00	91.0
235.00	318.0
235.90	102.0
237.10	99.0
246.90	56.0
249.00	2385.0
249.90	652.0
250.90	1128.0
252.10	301.0
252.90	182.0
265.00	3054.0
265.90	731.0
267.00	694.0
268.00	176.0
269.00	69.0
278.20	95.0
278.90	108.0
281.10	44632.0
282.00	11837.0
283.10	6997.0
284.10	1541.0
285.10	462.0

Instrument :
MSVOA_W
ClientSampleId :
BFB95