

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW103024\
 Data File : VW030829.D
 Acq On : 30 Oct 2024 12:04
 Operator : SY/MD
 Sample : VW1030SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 01 01:04:35 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Nov 01 01:03:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	335717	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	300490	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	126864	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	94161	17.844	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	71.360%
7) Chloroethane-d5	2.905	69	85750	21.467	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.880%
11) 1,1-Dichloroethene-d2	4.027	65	38525	17.553	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	70.200%
21) 2-Butanone-d5	7.075	46	41136	43.317	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.640%
24) Chloroform-d	7.740	84	294	0.031	ug/L	0.09
Spiked Amount	25.000	Range	40 - 150	Recovery	=	0.120%#
26) 1,2-Dichloroethane-d4	8.307	65	113036	22.641	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.560%
32) Benzene-d6	8.276	84	367840	21.091	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	84.360%
36) 1,2-Dichloropropane-d6	9.276	67	117004	22.857	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.440%
41) Toluene-d8	10.319	98	342234	21.496	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	86.000%
43) trans-1,3-Dichloroprop...	10.575	79	46917	21.888	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.560%
47) 2-Hexanone-d5	10.922	63	32028	48.578	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.160%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	86058	22.892	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	91.560%
66) 1,2-Dichlorobenzene-d4	13.849	152	109707	25.558	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.240%
Target Compounds						
39) cis-1,3-Dichloropropene	10.038	75	3963	0.538	ug/L	# 70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW103024\
Data File : VW030829.D
Acq On : 30 Oct 2024 12:04
Operator : SY/MD
Sample : VW1030SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Nov 01 01:04:35 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Nov 01 01:03:00 2024
Response via : Initial Calibration

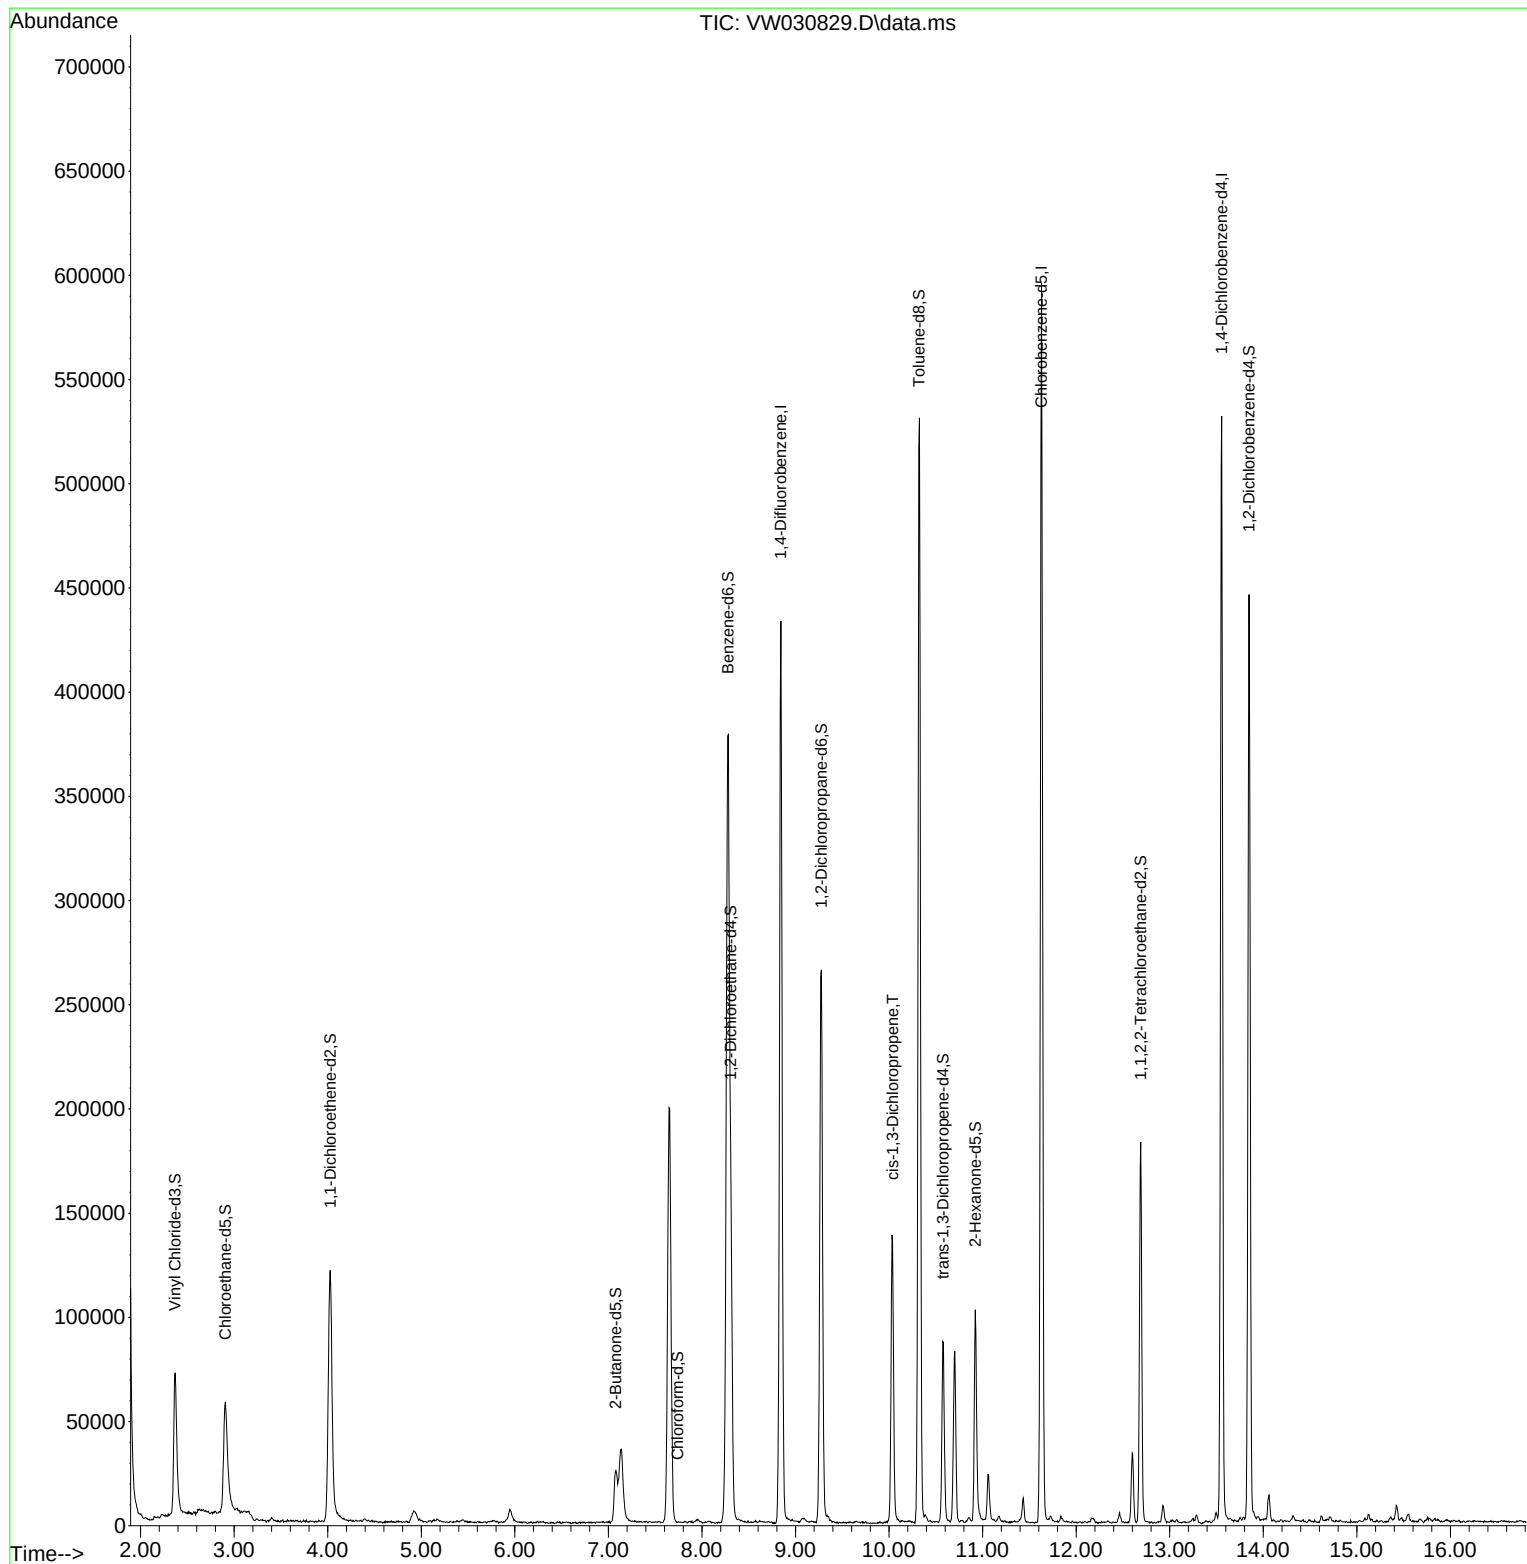

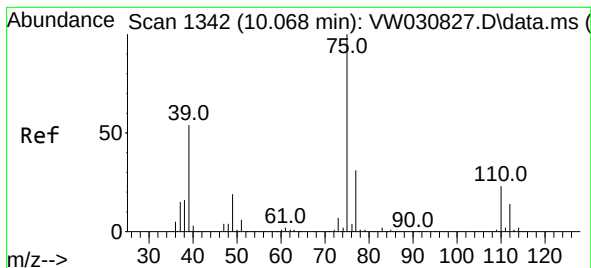

#39
 cis-1,3-Dichloropropene
 Concen: 0.538 ug/L
 RT: 10.038 min Scan# 11
 Delta R.T. -0.030 min
 Lab File: VW030829.D
 Acq: 30 Oct 2024 12:04

Instrument :
 MSVOA_W
 ClientSampleId :

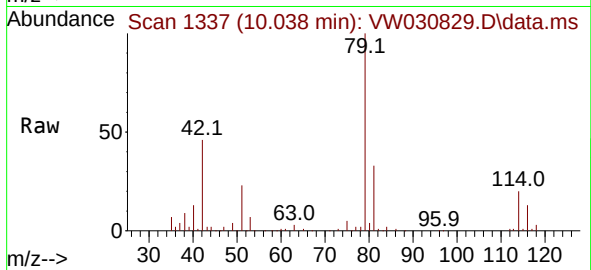

Tgt Ion: 75 Resp: 3963
 Ion Ratio Lower Upper
 75 100
 77 46.2 21.1 39.1#

