

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW103024\
 Data File : VW030833.D
 Acq On : 30 Oct 2024 13:52
 Operator : SY/MD
 Sample : P4494-04
 Misc : 5.00g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 01 01:05:21 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Nov 01 01:03:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	312055	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	283405	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	133541	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	80769	16.467	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	65.880%		
7) Chloroethane-d5	2.899	69	74194	19.983	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	79.920%		
11) 1,1-Dichloroethene-d2	4.021	65	32662	16.010	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	64.040%		
21) 2-Butanone-d5	7.075	46	38349	43.444	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	86.880%		
24) Chloroform-d	7.654	84	190505	21.347	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	85.400%		
26) 1,2-Dichloroethane-d4	8.307	65	98918	21.316	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	85.280%		
32) Benzene-d6	8.276	84	325426	19.784	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	79.120%		
36) 1,2-Dichloropropane-d6	9.270	67	107375	22.241	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	88.960%		
41) Toluene-d8	10.325	98	300749	20.029	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	80.120%		
43) trans-1,3-Dichloroprop...	10.575	79	40499	20.033	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	80.120%		
47) 2-Hexanone-d5	10.922	63	28914	46.498	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	93.000%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	88530	24.969	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	99.880%		
66) 1,2-Dichlorobenzene-d4	13.849	152	103115	22.821	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	91.280%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.038	75	3378	0.486	ug/L	# 70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW103024\
Data File : VW030833.D
Acq On : 30 Oct 2024 13:52
Operator : SY/MD
Sample : P4494-04
Misc : 5.00g/10mL/MSVOA_W/SOIL/A
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Nov 01 01:05:21 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Nov 01 01:03:00 2024
Response via : Initial Calibration

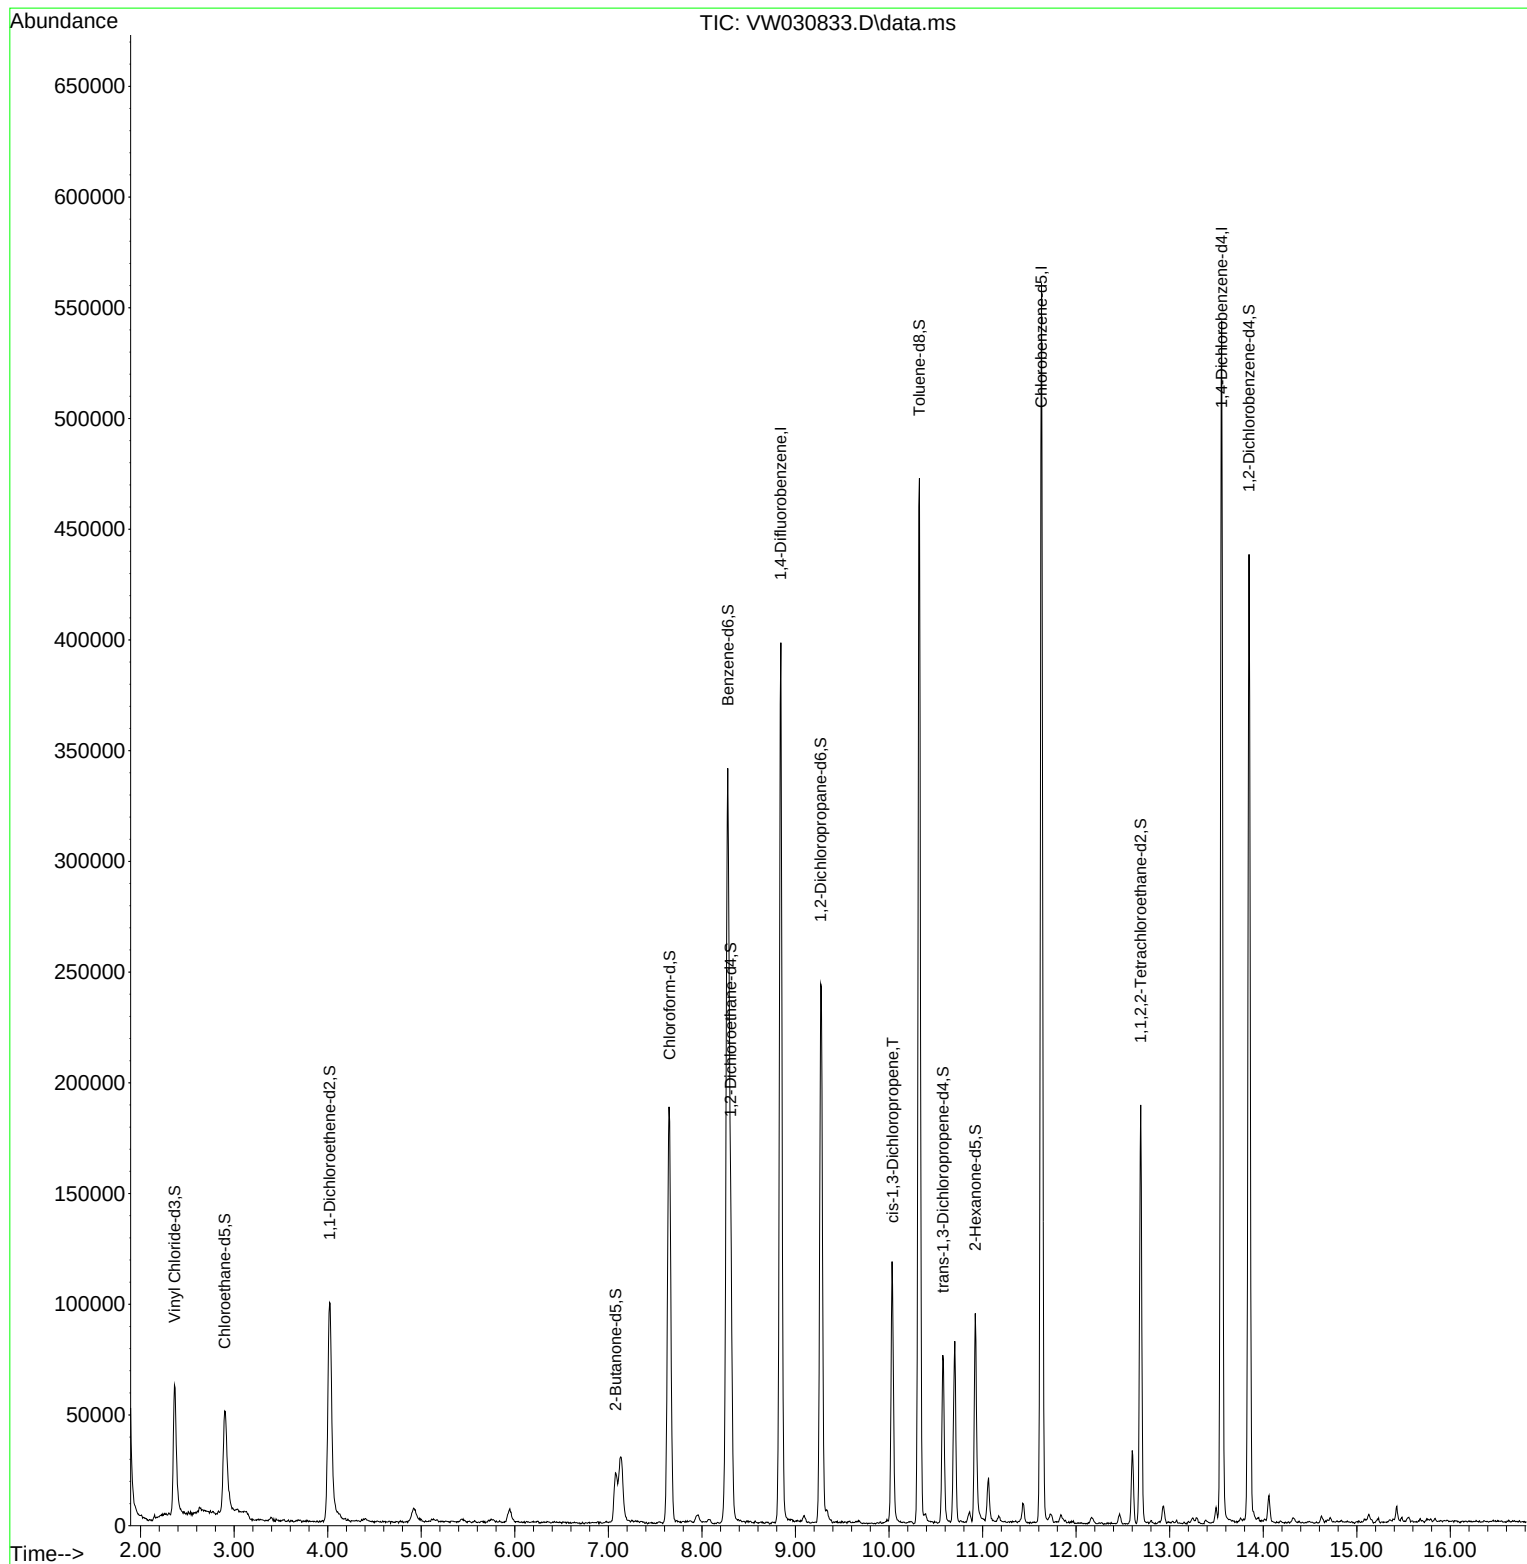

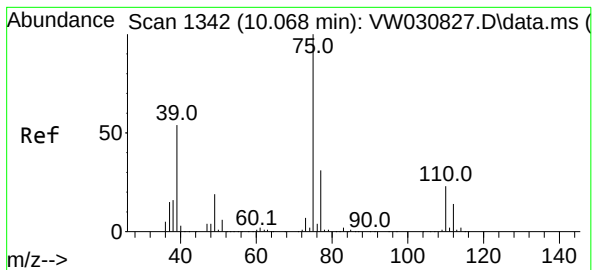

#39
 cis-1,3-Dichloropropene
 Concen: 0.486 ug/L
 RT: 10.038 min Scan# 11
 Delta R.T. -0.030 min
 Lab File: VW030833.D
 Acq: 30 Oct 2024 13:52

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75	Resp:	3378
Ion Ratio	Lower	Upper
75	100	
77	46.2	21.1 39.1#

