

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW103024\
 Data File : VW030835.D
 Acq On : 30 Oct 2024 14:50
 Operator : SY/MD
 Sample : P4568-19
 Misc : 5.13g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 01 01:05:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Nov 01 01:03:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	318647	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	317862	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	125291	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	92765	18.521	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.080%
7) Chloroethane-d5	2.899	69	90730	23.931	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.720%
11) 1,1-Dichloroethene-d2	4.021	65	38697	18.576	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	74.320%
21) 2-Butanone-d5	7.075	46	42781	47.462	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.920%
24) Chloroform-d	7.648	84	209353	22.974	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.880%
26) 1,2-Dichloroethane-d4	8.307	65	113913	24.039	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.160%
32) Benzene-d6	8.276	84	390363	21.159	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	84.640%
36) 1,2-Dichloropropane-d6	9.270	67	120032	22.167	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	88.680%
41) Toluene-d8	10.325	98	367898	21.845	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.360%
43) trans-1,3-Dichloroprop...	10.581	79	50880	22.440	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.760%
47) 2-Hexanone-d5	10.922	63	37906	54.351	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	108.700%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	97666	24.560	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	98.240%
66) 1,2-Dichlorobenzene-d4	13.855	152	114968	27.119	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	108.480%
Target Compounds						
39) cis-1,3-Dichloropropene	10.032	75	4377	0.562	ug/L	Qvalue # 68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW103024\
Data File : VW030835.D
Acq On : 30 Oct 2024 14:50
Operator : SY/MD
Sample : P4568-19
Misc : 5.13g/10mL/MSVOA_W/SOIL/B
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Nov 01 01:05:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Nov 01 01:03:00 2024
Response via : Initial Calibration

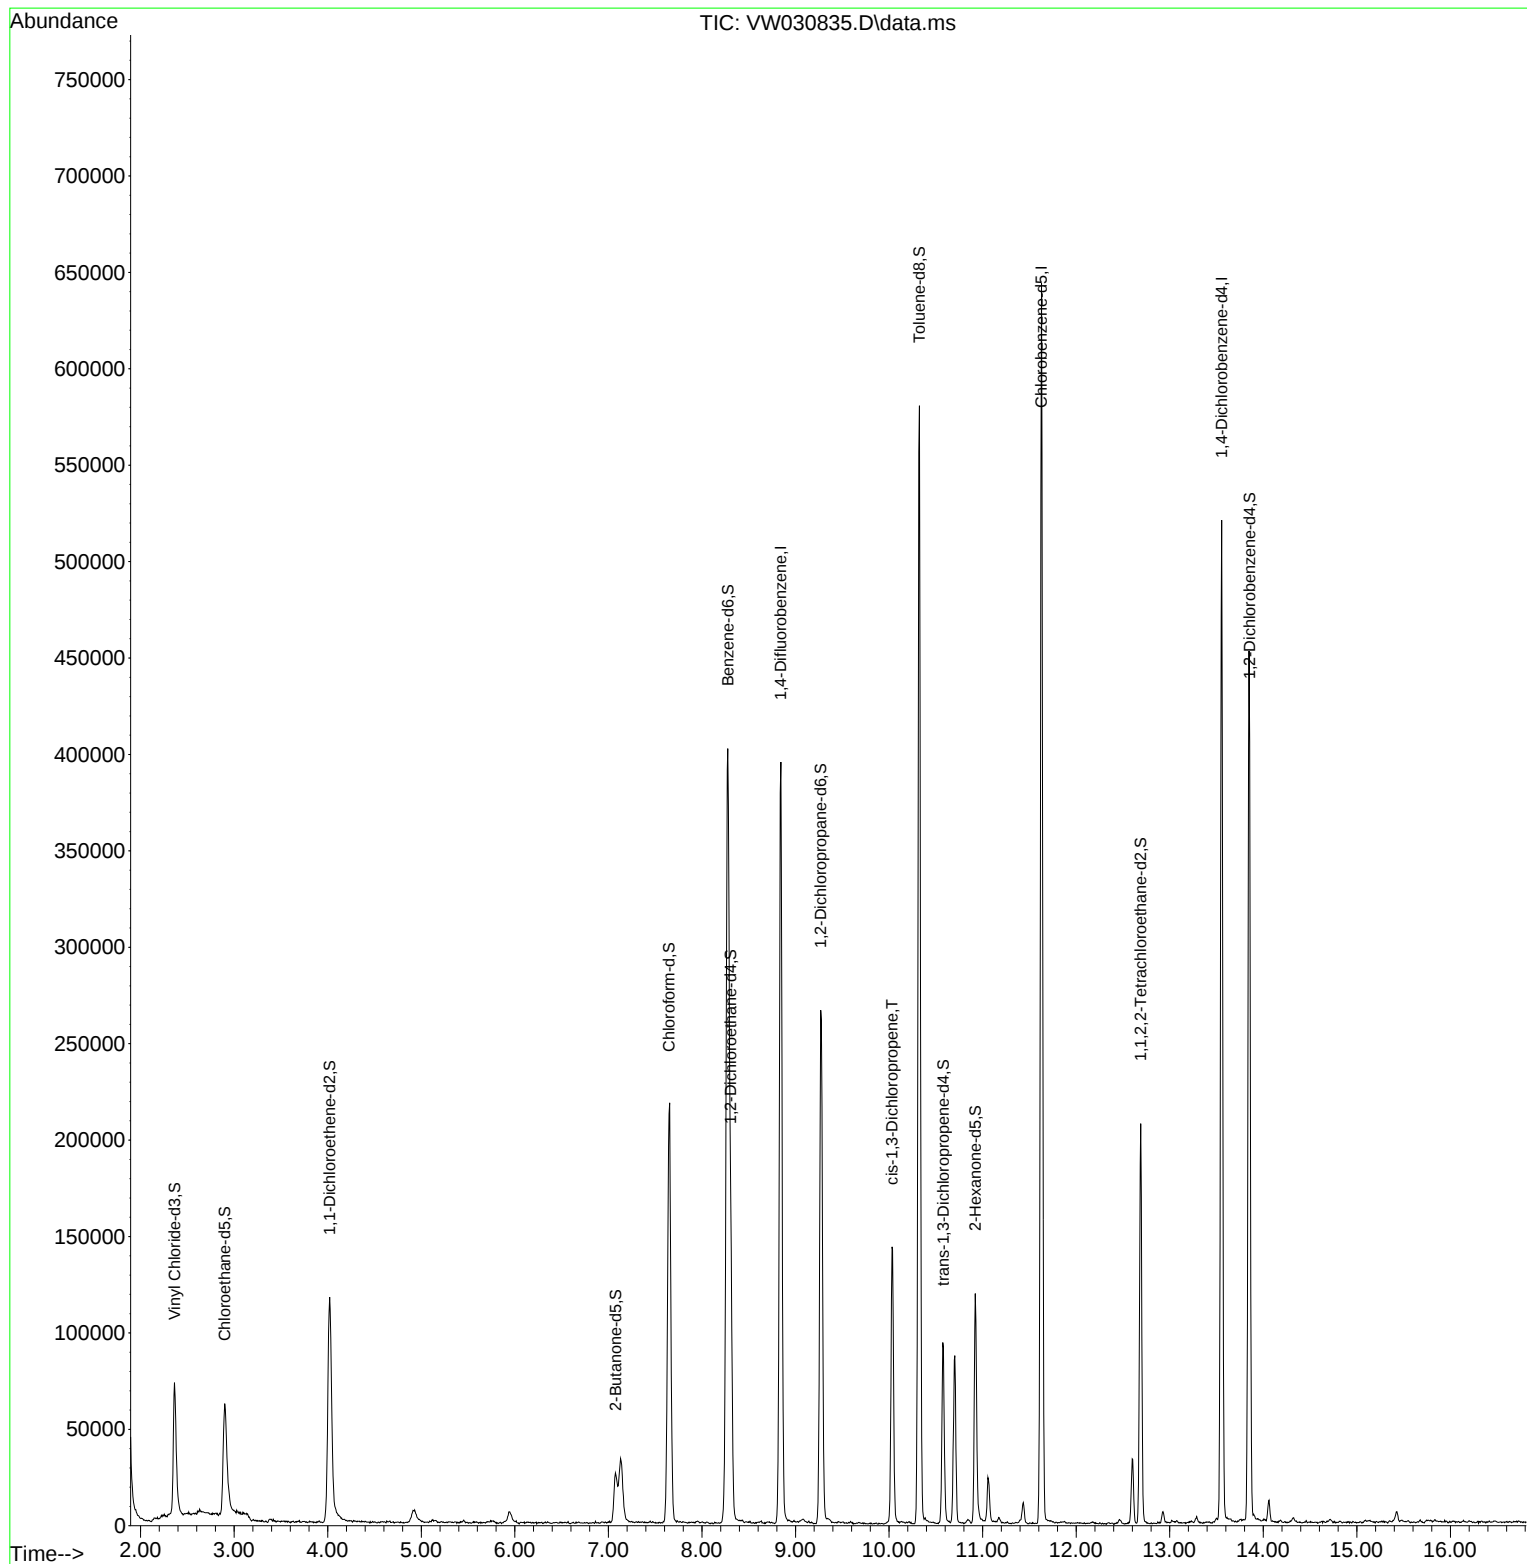

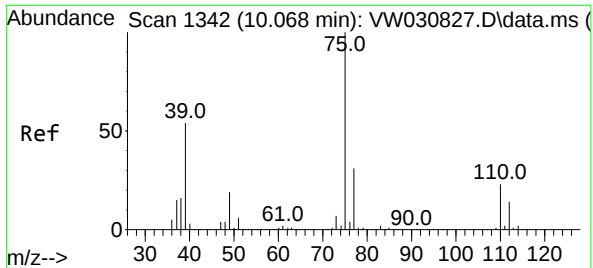

#39
 cis-1,3-Dichloropropene
 Concen: 0.562 ug/L
 RT: 10.032 min Scan# 11
 Delta R.T. -0.036 min
 Lab File: VW030835.D
 Acq: 30 Oct 2024 14:50

Instrument :
 MSVOA_W
 ClientSampleId :

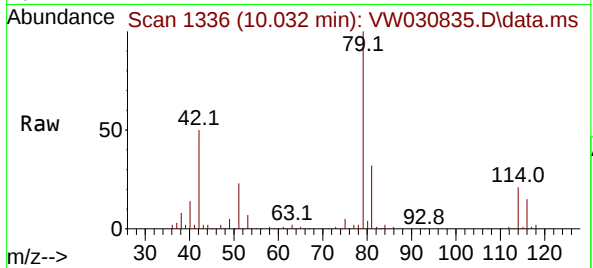

Tgt Ion: 75 Resp: 4377
 Ion Ratio Lower Upper
 75 100
 77 47.2 21.1 39.1#

