

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW103024\
 Data File : VW030836.D
 Acq On : 30 Oct 2024 15:14
 Operator : SY/MD
 Sample : P4568-20
 Misc : 4.76g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 01 01:05:58 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Nov 01 01:03:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	313066	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	289101	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	127650	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	86647	17.608	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.440%
7) Chloroethane-d5	3.058	69	440	0.118	ug/L	0.16
Spiked Amount	25.000	Range	30 - 150	Recovery	=	0.480%#
11) 1,1-Dichloroethene-d2	4.021	65	33775	16.502	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.000%
21) 2-Butanone-d5	7.075	46	38885	43.909	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.820%
24) Chloroform-d	7.648	84	180045	20.110	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	80.440%
26) 1,2-Dichloroethane-d4	8.307	65	109964	23.620	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	94.480%
32) Benzene-d6	8.276	84	353846	21.088	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	84.360%
36) 1,2-Dichloropropane-d6	9.276	67	103790	21.075	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	84.280%
41) Toluene-d8	10.319	98	284050	18.544	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	74.160%
43) trans-1,3-Dichloroprop...	10.581	79	39265	19.040	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	76.160%
47) 2-Hexanone-d5	10.922	63	29850	47.058	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.120%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	80480	22.251	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	89.000%
66) 1,2-Dichlorobenzene-d4	13.848	152	97873	22.660	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.640%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.038	75	3163	0.446	ug/L	# 76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW103024\
Data File : VW030836.D
Acq On : 30 Oct 2024 15:14
Operator : SY/MD
Sample : P4568-20
Misc : 4.76g/10mL/MSVOA_W/SOIL/B
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Nov 01 01:05:58 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Nov 01 01:03:00 2024
Response via : Initial Calibration

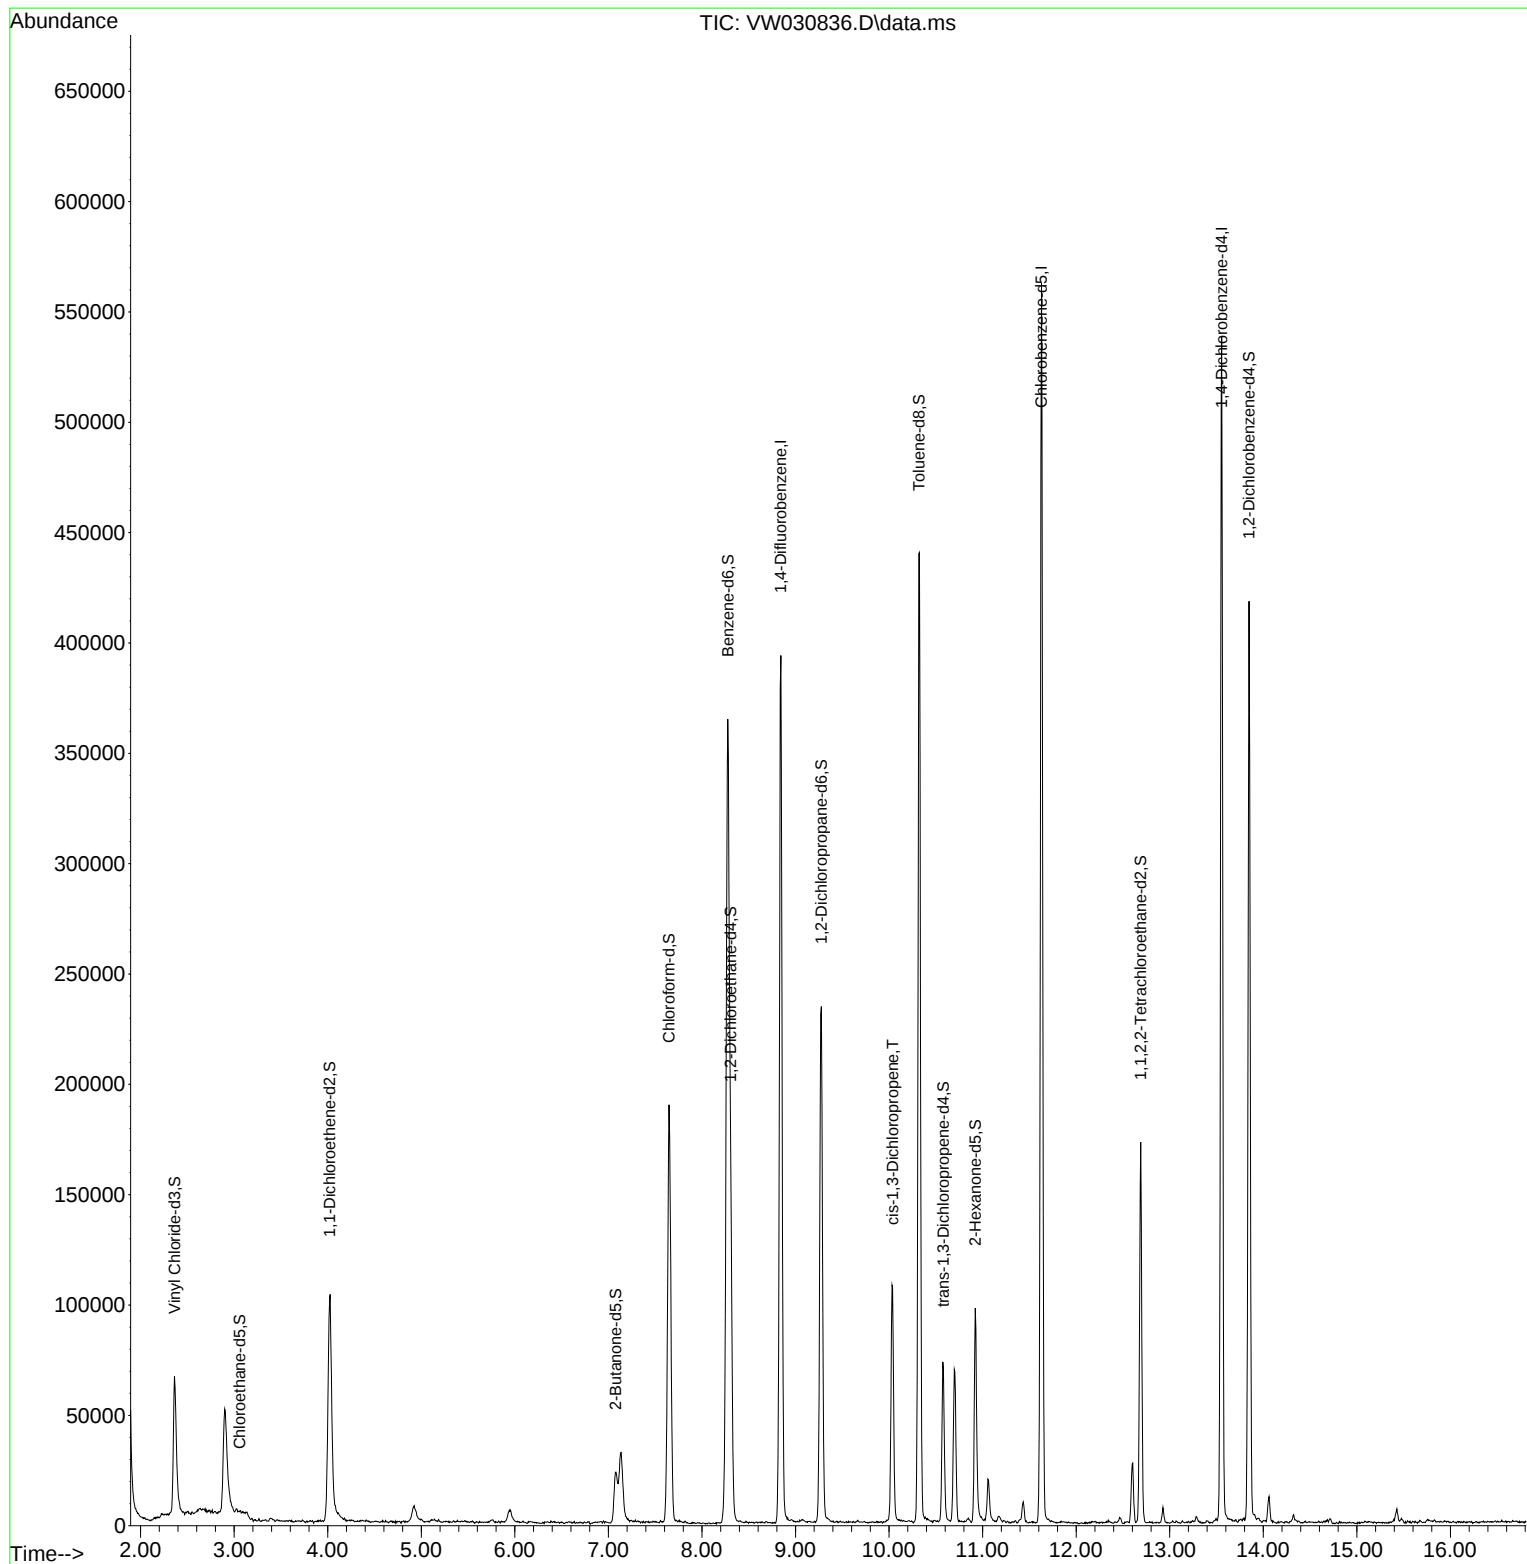

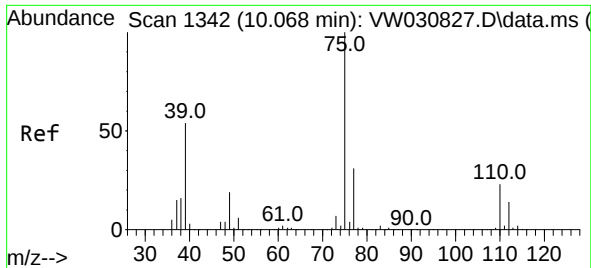

#39
 cis-1,3-Dichloropropene
 Concen: 0.446 ug/L
 RT: 10.038 min Scan# 11
 Delta R.T. -0.030 min
 Lab File: VW030836.D
 Acq: 30 Oct 2024 15:14

Instrument :
 MSVOA_W
 ClientSampleId :

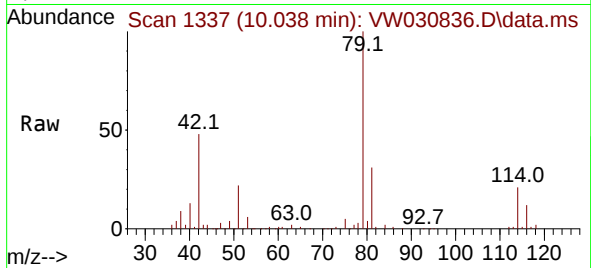

Tgt Ion: 75 Resp: 3163
 Ion Ratio Lower Upper
 75 100
 77 42.9 21.1 39.1#

