

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW103024\
 Data File : VW030841.D
 Acq On : 30 Oct 2024 17:14
 Operator : SY/MD
 Sample : P4581-09
 Misc : 4.53g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 01 01:06:58 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Nov 01 01:03:00 2024
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		8.843	114	84894	25.000	ug/L	0.00
28) Chlorobenzene-d5		11.629	117	89531	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.556	152	35719	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.363	65	36140	27.083	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 108.320%		
7) Chloroethane-d5		2.899	69	32293	31.970	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 127.880%		
11) 1,1-Dichloroethene-d2		4.027	65	13581	24.470	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	= 97.880%		
21) 2-Butanone-d5		7.081	46	9031	37.607	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	= 75.220%		
24) Chloroform-d		7.648	84	73097	30.108	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	= 120.440%		
26) 1,2-Dichloroethane-d4		8.307	65	37469	29.679	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	= 118.720%		
32) Benzene-d6		8.276	84	114870	22.106	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	= 88.440%		
36) 1,2-Dichloropropane-d6		9.270	67	37887	24.841	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	= 99.360%		
41) Toluene-d8		10.325	98	93708	19.754	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	= 79.000%		
43) trans-1,3-Dichloroprop...		10.574	79	13126	20.553	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	= 82.200%		
47) 2-Hexanone-d5		10.922	63	6461	32.890	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	= 65.780%		
56) 1,1,2,2-Tetrachloroeth...		12.690	84	30369	27.113	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	= 108.440%		
66) 1,2-Dichlorobenzene-d4		13.848	152	29962	24.791	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	= 99.160%		
Target Compounds							Qvalue
39) cis-1,3-Dichloropropene		10.044	75	1323	0.603	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW103024\
Data File : VW030841.D
Acq On : 30 Oct 2024 17:14
Operator : SY/MD
Sample : P4581-09
Misc : 4.53g/10mL/MSVOA_W/SOIL/A
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Nov 01 01:06:58 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Nov 01 01:03:00 2024
Response via : Initial Calibration

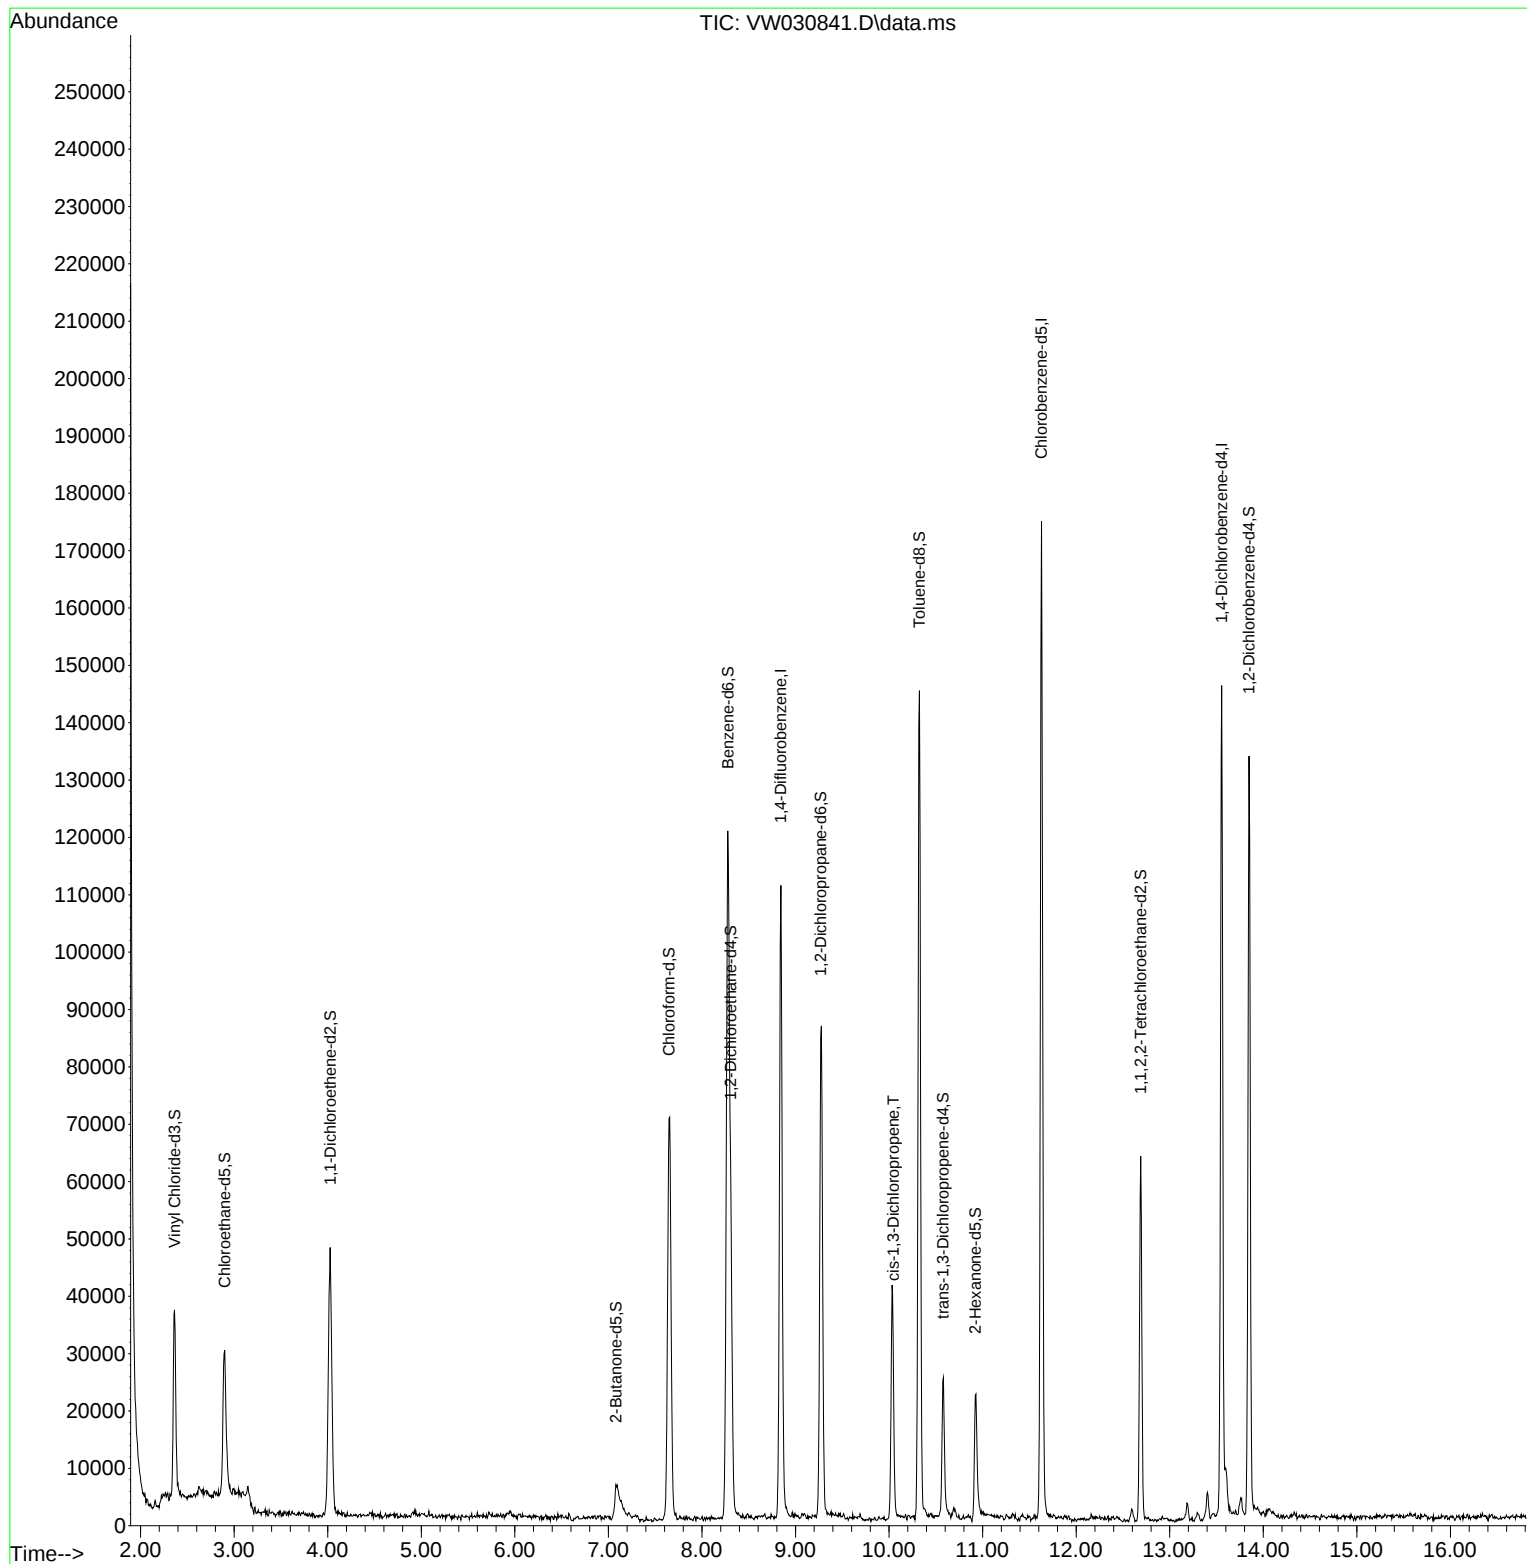

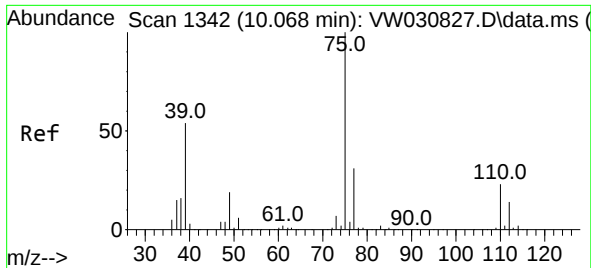

#39
 cis-1,3-Dichloropropene
 Concen: 0.603 ug/L
 RT: 10.044 min Scan# 11
 Delta R.T. -0.024 min
 Lab File: VW030841.D
 Acq: 30 Oct 2024 17:14

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 1323
 Ion Ratio Lower Upper
 75 100
 77 31.4 21.1 39.1

