

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW103024\
 Data File : VW030845.D
 Acq On : 30 Oct 2024 18:50
 Operator : SY/MD
 Sample : P4581-13
 Misc : 4.27g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 01 01:07:45 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Nov 01 01:03:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	79043	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	87068	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	32766	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	23792	19.149	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.600%
7) Chloroethane-d5	2.893	69	24380	25.923	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	103.680%
11) 1,1-Dichloroethene-d2	4.027	65	8940	17.300	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	69.200%
21) 2-Butanone-d5	7.087	46	8532	38.159	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	76.320%
24) Chloroform-d	7.654	84	55269	24.450	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.800%
26) 1,2-Dichloroethane-d4	8.307	65	36359	30.932	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	123.720%
32) Benzene-d6	8.276	84	98242	19.441	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	77.760%
36) 1,2-Dichloropropane-d6	9.270	67	32014	21.584	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	86.320%
41) Toluene-d8	10.325	98	79396	17.211	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	68.840%
43) trans-1,3-Dichloroprop...	10.575	79	12624	20.326	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	81.320%
47) 2-Hexanone-d5	10.928	63	6958	36.422	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	72.840%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	27691	25.421	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	101.680%
66) 1,2-Dichlorobenzene-d4	13.848	152	27920	25.183	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.720%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	972	0.455	ug/L	# 60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW103024\
Data File : VW030845.D
Acq On : 30 Oct 2024 18:50
Operator : SY/MD
Sample : P4581-13
Misc : 4.27g/10mL/MSVOA_W/SOIL/A
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Nov 01 01:07:45 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Nov 01 01:03:00 2024
Response via : Initial Calibration

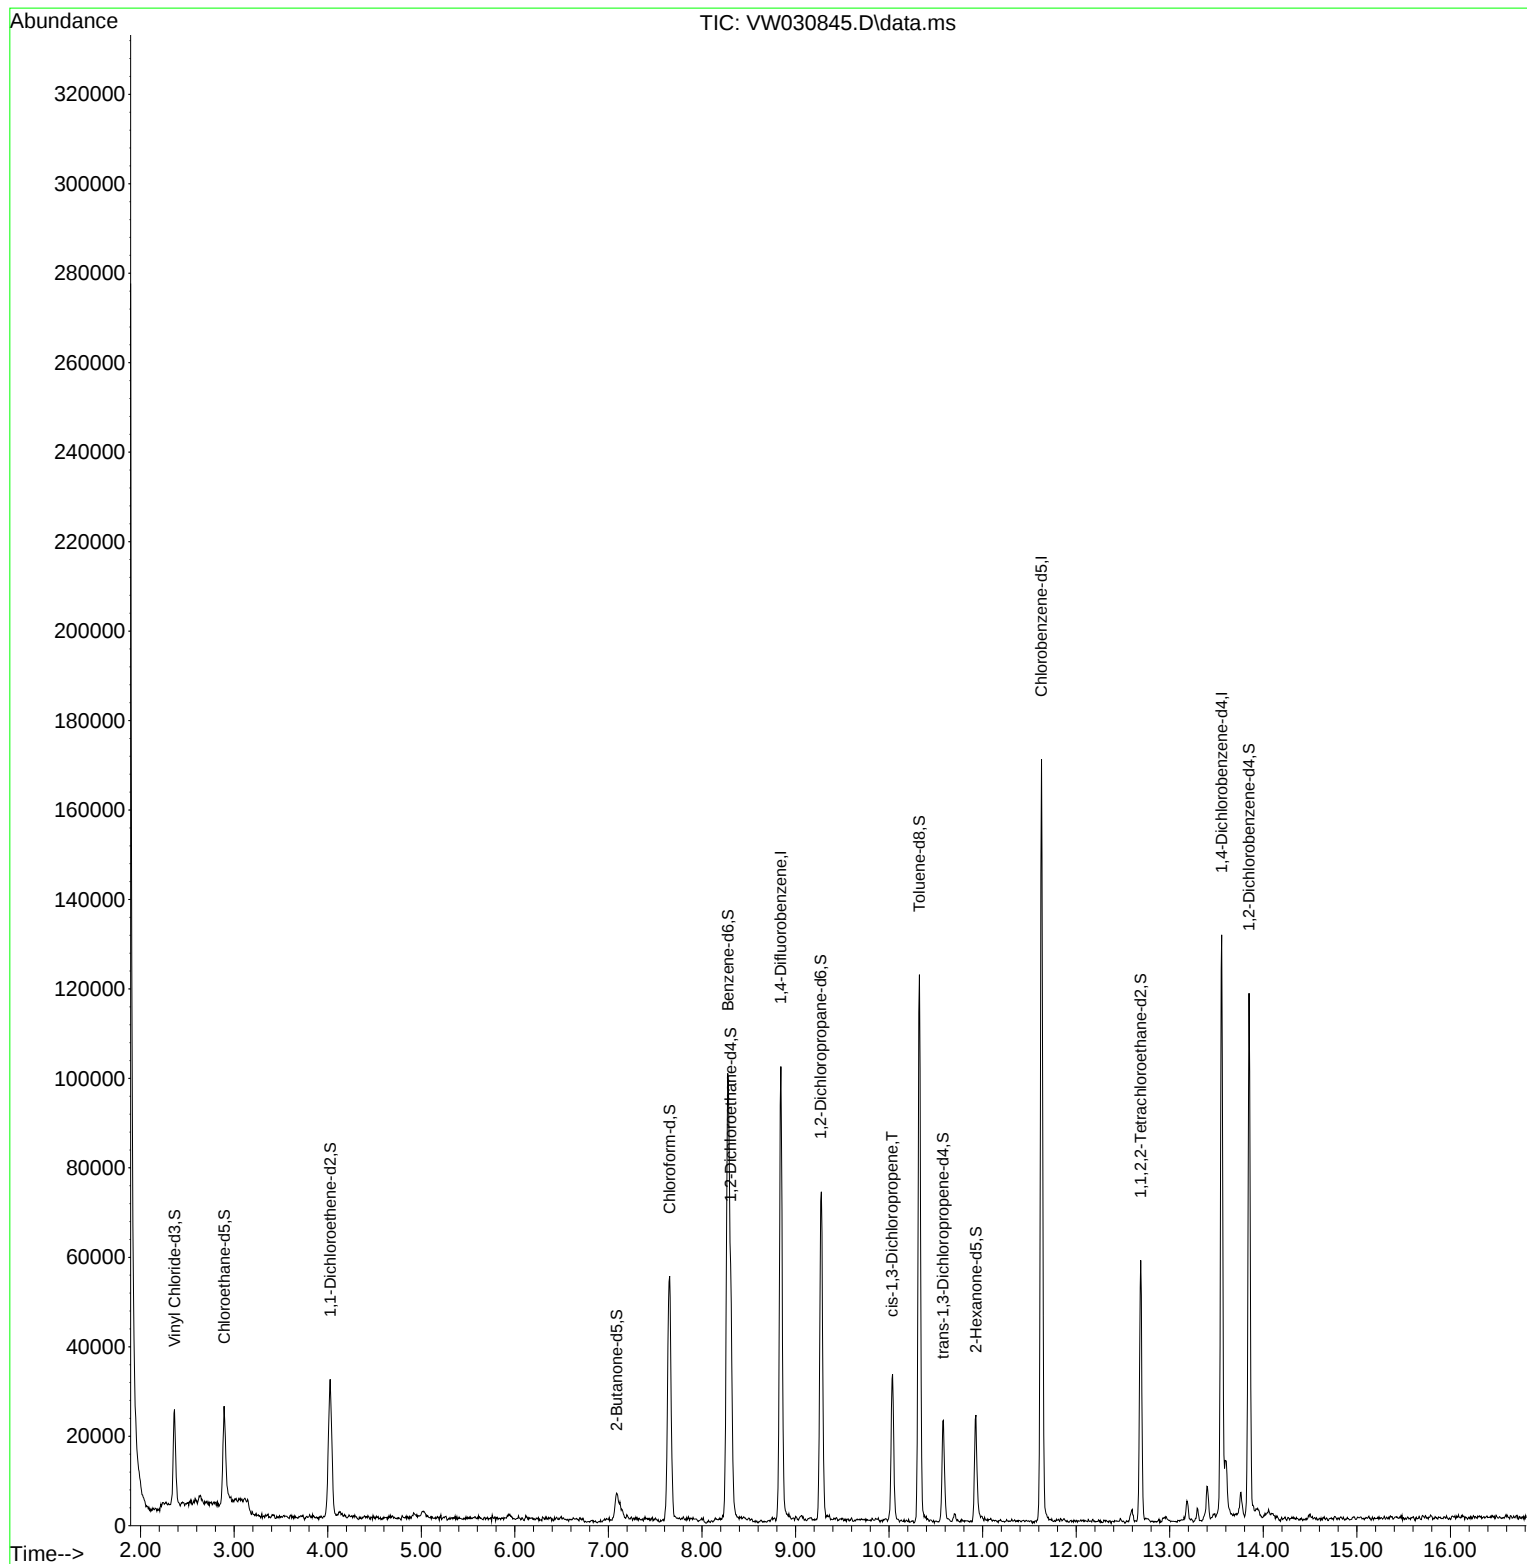

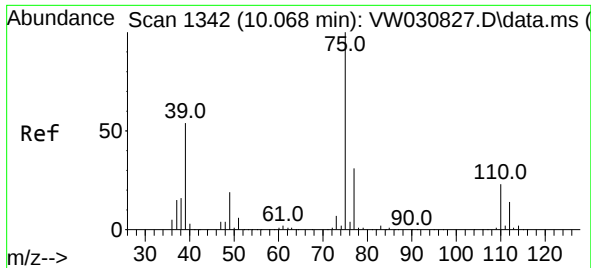

#39

cis-1,3-Dichloropropene

Concen: 0.455 ug/L

RT: 10.032 min Scan# 11

Delta R.T. -0.037 min


Lab File: VW030845.D

Acq: 30 Oct 2024 18:50

Instrument :

MSVOA_W

ClientSampleId :

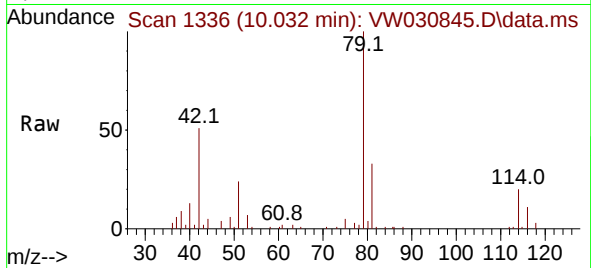

Tgt Ion: 75 Resp: 972

Ion Ratio Lower Upper

75 100

77 51.9 21.1 39.1#

