

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW103124\
 Data File : VW030851.D
 Acq On : 31 Oct 2024 11:13
 Operator : SY/MD
 Sample : P4581-15
 Misc : 4.21g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 01 03:11:23 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Nov 01 03:09:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	445686	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	400841	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	192572	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	160422	22.899	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.600%
7) Chloroethane-d5	2.905	69	136337	25.710	ug/L	0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	102.840%
11) 1,1-Dichloroethene-d2	4.021	65	67357	23.117	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	92.480%
21) 2-Butanone-d5	7.075	46	38725	30.716	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	61.440%
24) Chloroform-d	7.648	84	282947	22.199	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.800%
26) 1,2-Dichloroethane-d4	8.307	65	151455	22.852	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.400%
32) Benzene-d6	8.276	84	595301	25.588	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	102.360%
36) 1,2-Dichloropropane-d6	9.270	67	156427	22.908	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.640%
41) Toluene-d8	10.325	98	555749	26.168	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	104.680%
43) trans-1,3-Dichloroprop...	10.575	79	57394	20.073	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	80.280%
47) 2-Hexanone-d5	10.922	63	29104	33.092	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	66.180%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	102100	20.360	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	81.440%
66) 1,2-Dichlorobenzene-d4	13.848	152	150381	23.079	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	92.320%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	5250	0.534	ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW103124\
Data File : VW030851.D
Acq On : 31 Oct 2024 11:13
Operator : SY/MD
Sample : P4581-15
Misc : 4.21g/10mL/MSVOA_W/SOIL/A
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Nov 01 03:11:23 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Nov 01 03:09:59 2024
Response via : Initial Calibration

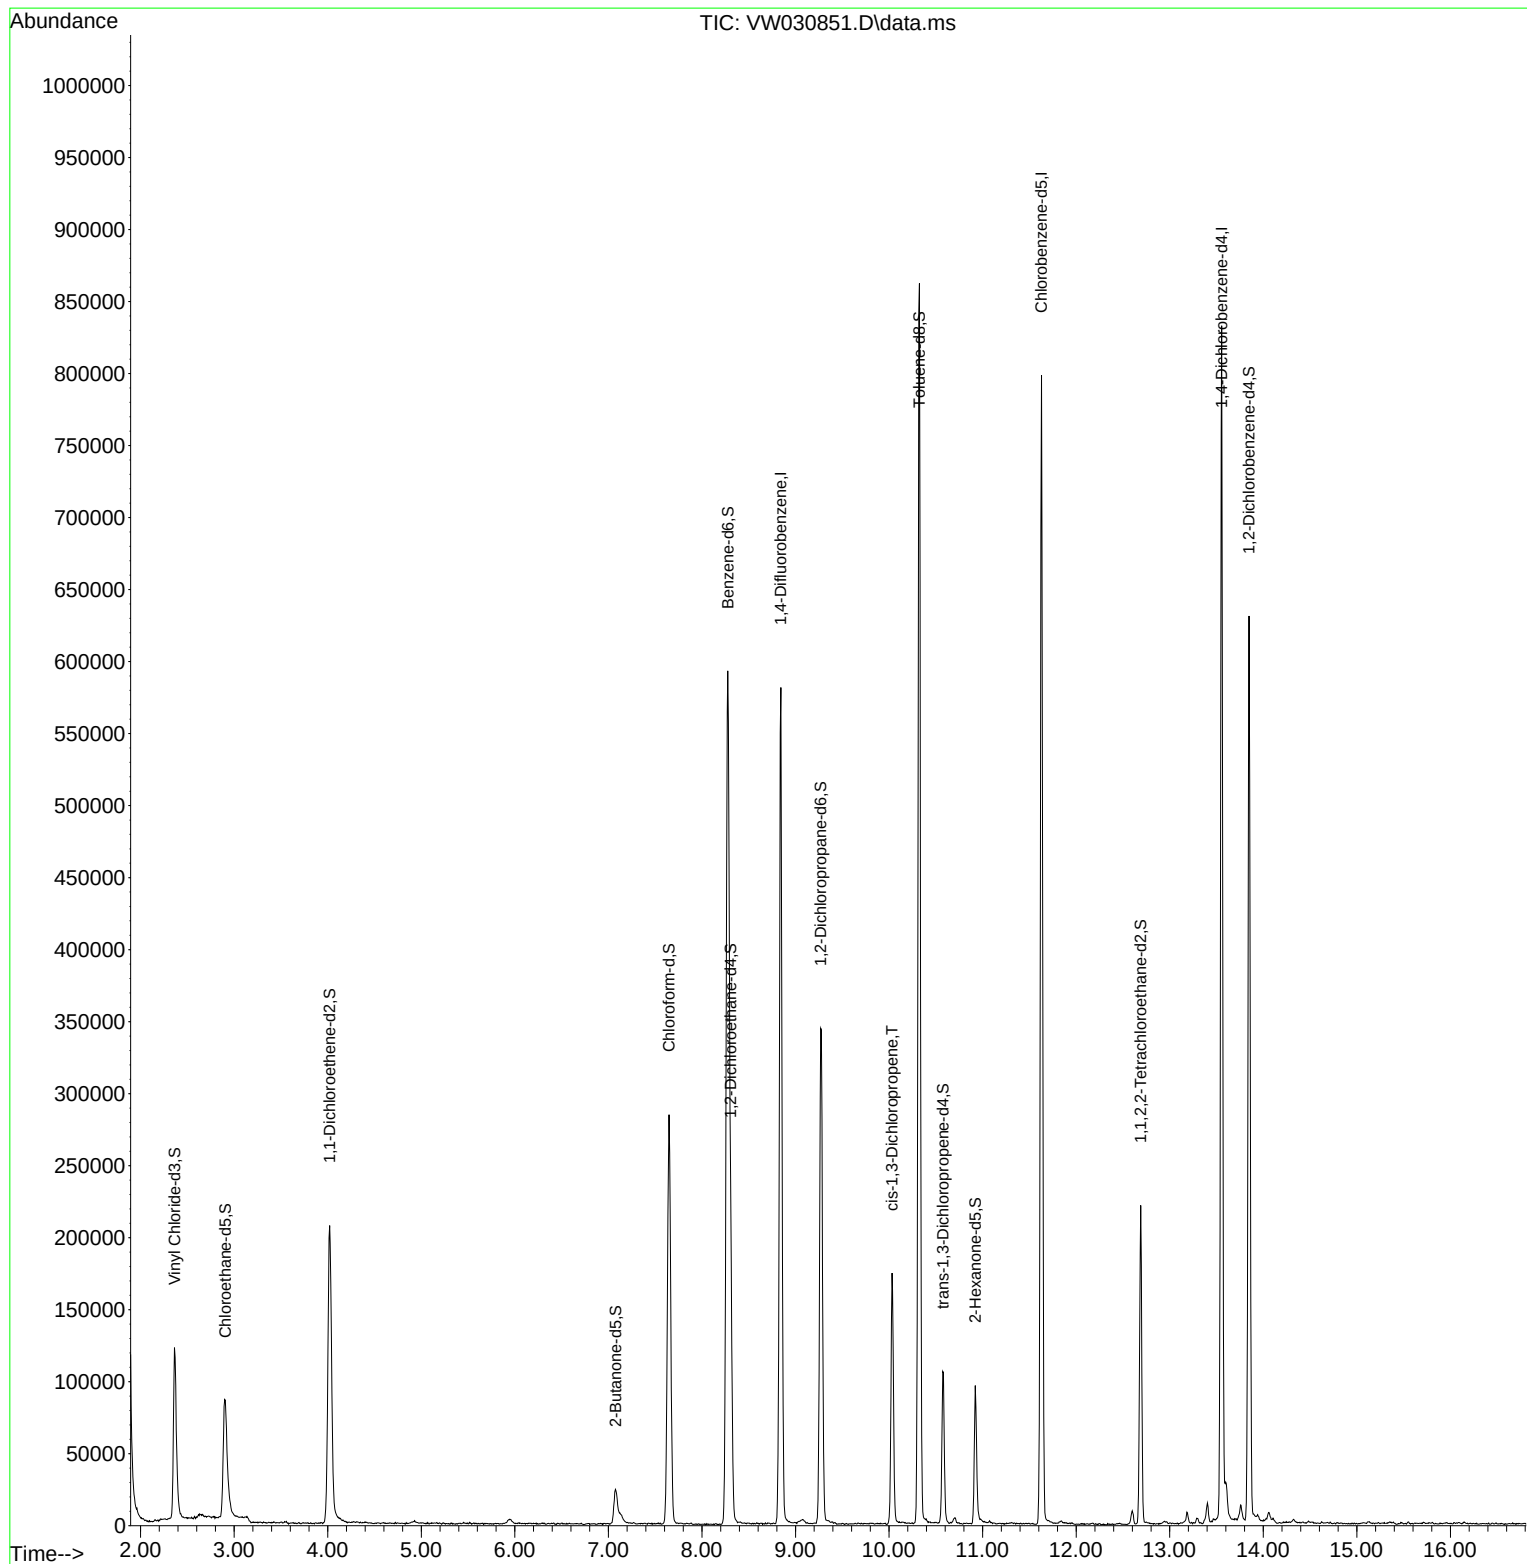

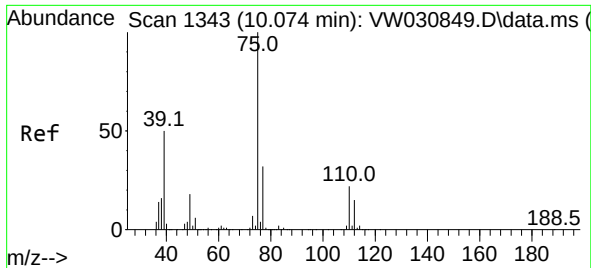

#39

cis-1,3-Dichloropropene

Concen: 0.534 ug/L

RT: 10.032 min Scan# 11

Delta R.T. -0.042 min


Lab File: VW030851.D

Acq: 31 Oct 2024 11:13

Instrument :

MSVOA_W

ClientSampleId :

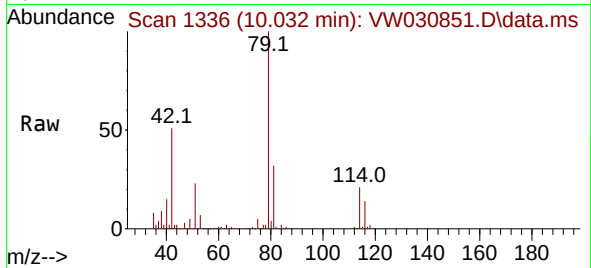

Tgt Ion: 75 Resp: 5250

Ion Ratio Lower Upper

75 100

77 38.3 21.1 39.1

