

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW103124\
 Data File : VW030855.D
 Acq On : 31 Oct 2024 12:49
 Operator : SY/MD
 Sample : P4581-13
 Misc : 5.09g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 01 03:12:21 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Nov 01 03:09:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	310600	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	319545	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	128730	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	77646	15.904	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	63.600%
7) Chloroethane-d5	2.899	69	67476	18.259	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	73.040%
11) 1,1-Dichloroethene-d2	4.021	65	29157	14.359	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.440%
21) 2-Butanone-d5	7.075	46	38042	43.298	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.600%
24) Chloroform-d	7.648	84	171815	19.343	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	77.360%
26) 1,2-Dichloroethane-d4	8.307	65	102935	22.286	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	89.160%
32) Benzene-d6	8.276	84	326887	17.625	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	70.520%
36) 1,2-Dichloropropane-d6	9.276	67	100756	18.509	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	74.040%
41) Toluene-d8	10.325	98	289109	17.076	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	68.320%
43) trans-1,3-Dichloroprop...	10.581	79	39758	17.442	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	69.760%
47) 2-Hexanone-d5	10.922	63	28293	40.354	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	80.700%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	82553	20.650	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	82.600%
66) 1,2-Dichlorobenzene-d4	13.849	152	93871	21.551	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	86.200%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	3217	0.411	ug/L	# 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW103124\
Data File : VW030855.D
Acq On : 31 Oct 2024 12:49
Operator : SY/MD
Sample : P4581-13
Misc : 5.09g/10mL/MSVOA_W/SOIL/B
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Nov 01 03:12:21 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Nov 01 03:09:59 2024
Response via : Initial Calibration

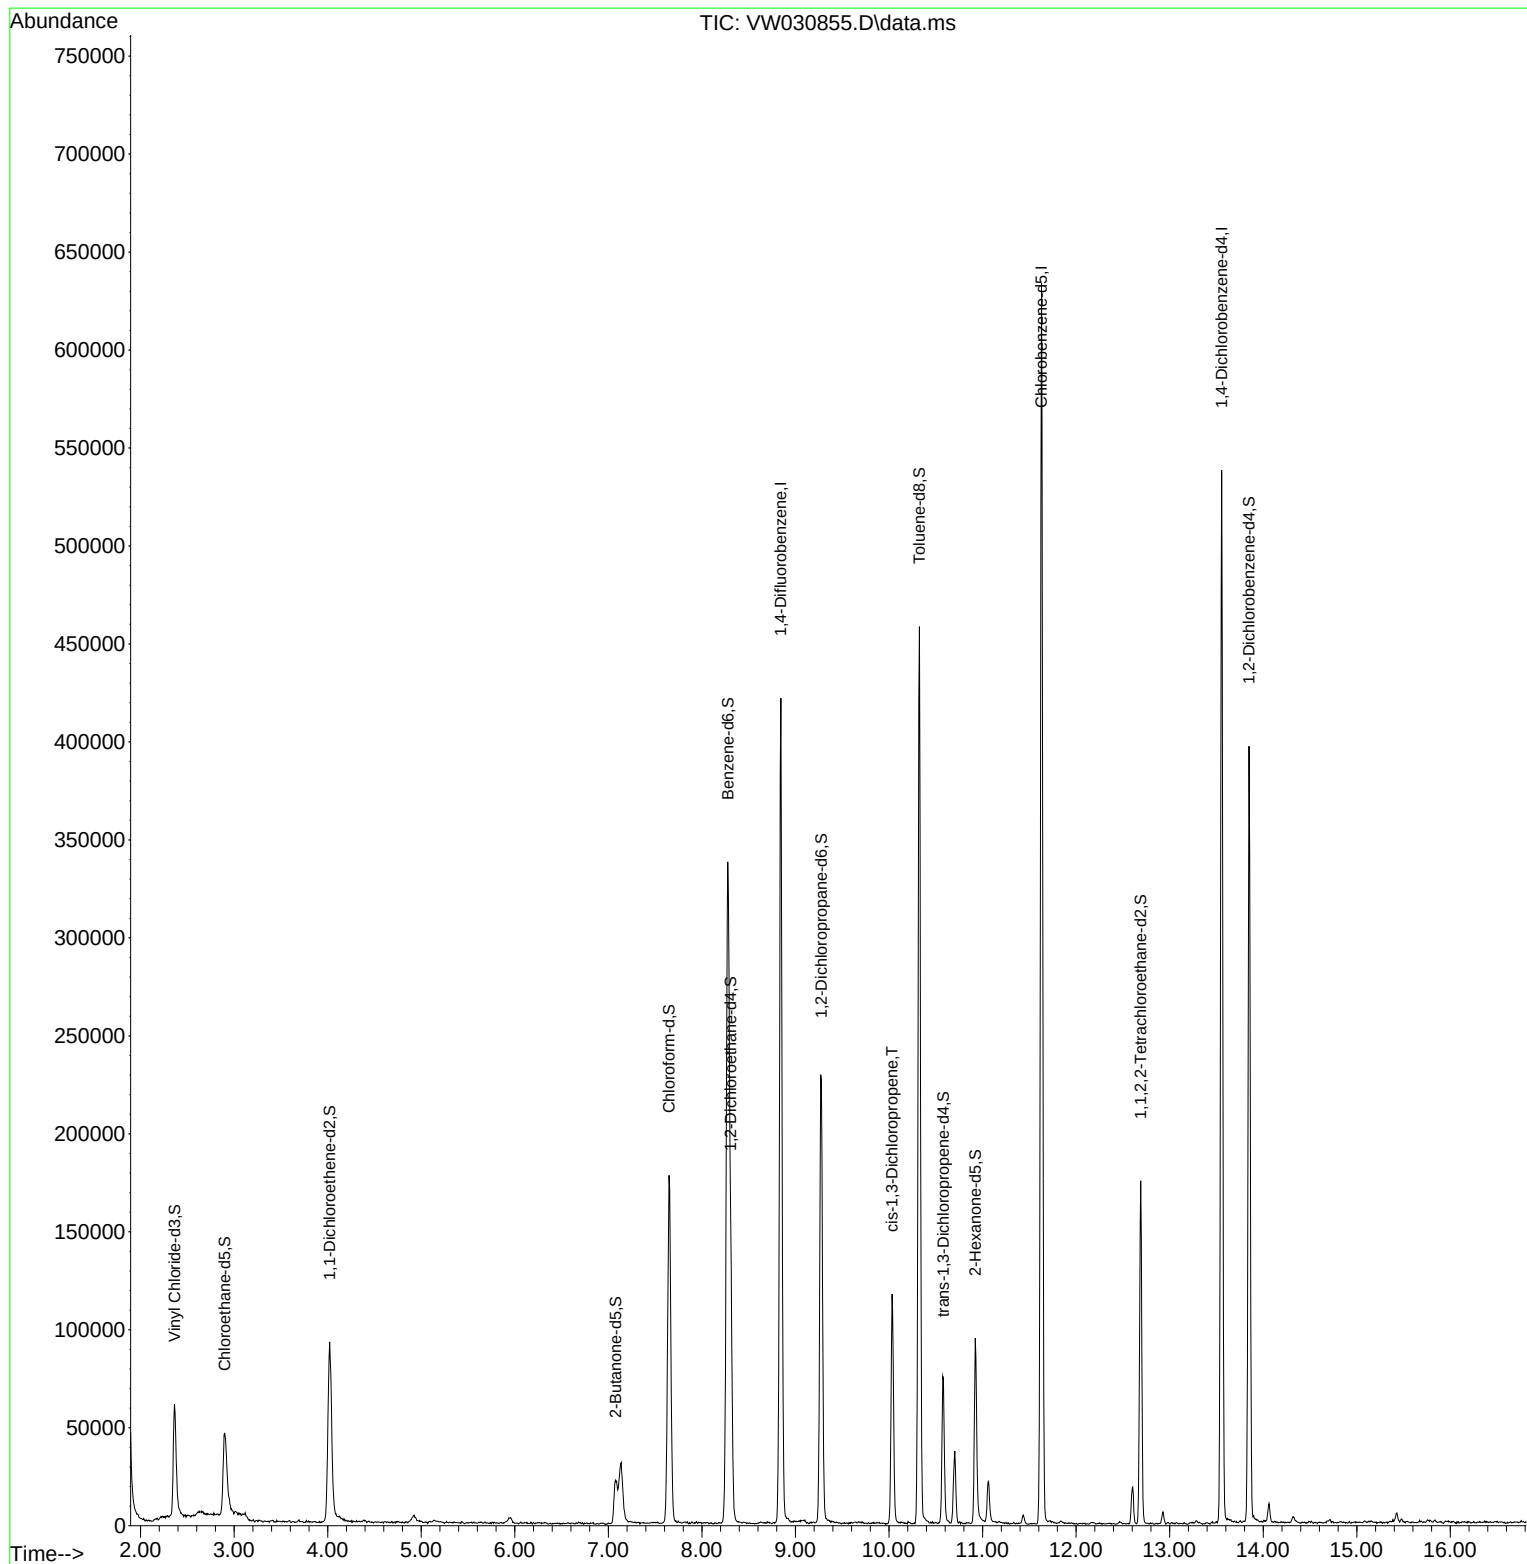

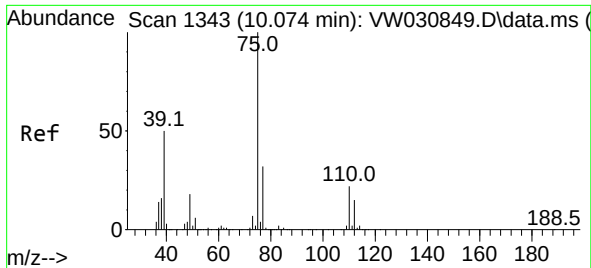

#39
 cis-1,3-Dichloropropene
 Concen: 0.411 ug/L
 RT: 10.032 min Scan# 11
 Delta R.T. -0.042 min
 Lab File: VW030855.D
 Acq: 31 Oct 2024 12:49

Instrument :
 MSVOA_W
 ClientSampleId :

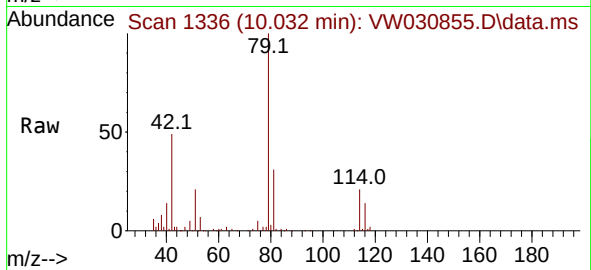

Tgt Ion: 75 Resp: 3217
 Ion Ratio Lower Upper
 75 100
 77 46.8 21.1 39.1#

