




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110123\
 Data File : VW027504.D
 Acq On : 01 Nov 2023 15:53
 Operator : SY/MD
 Sample : VIBLK564
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK564

Manual IntegrationsAPPROVED

Quant Time: Nov 02 03:37:06 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Nov 02 03:33:34 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 11/02/2023
 Supervised By :Mahesh Dadoda 11/02/2023

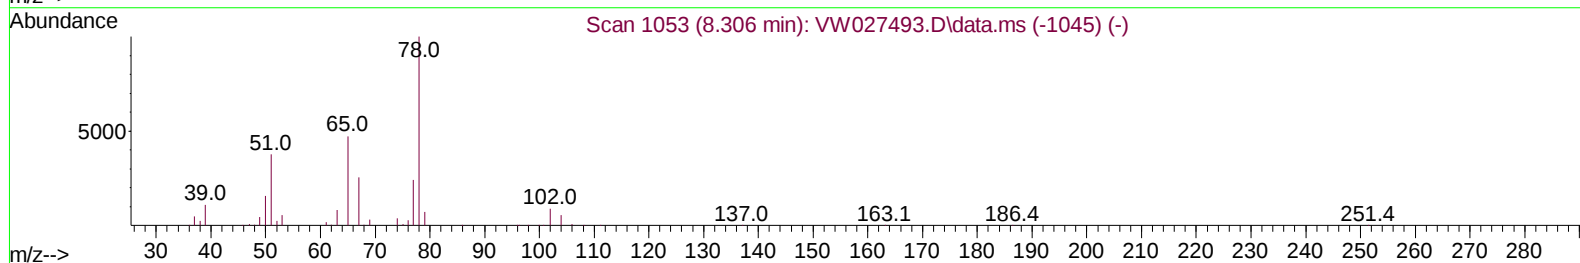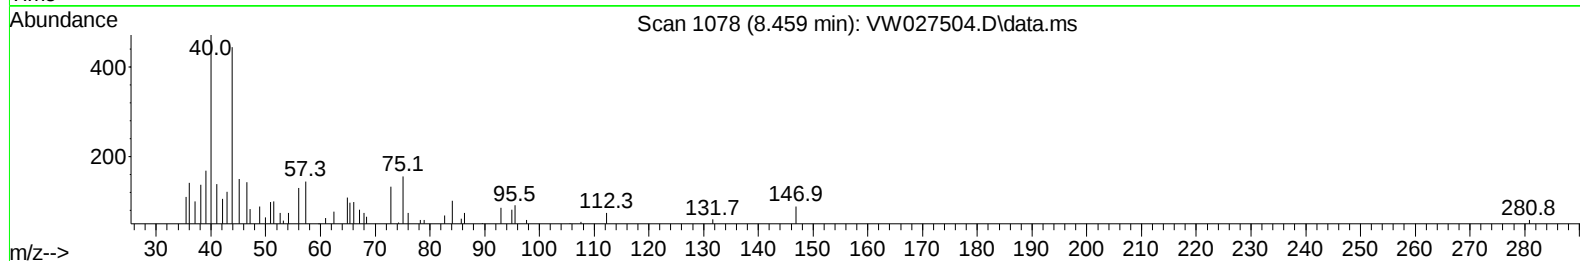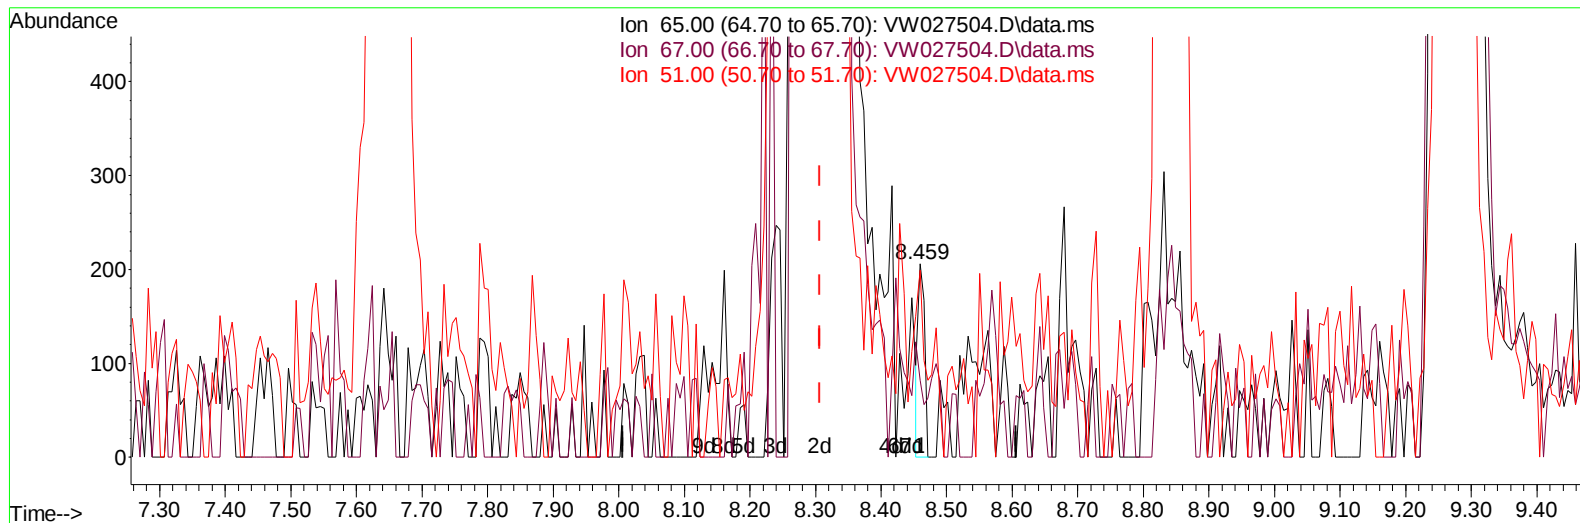

TIC: VW027504.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.459min (+ 0.153) 0.03 ug/L

response 137

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.00	57.66
51.00	99.60	94.16
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110123\
 Data File : VW027504.D
 Acq On : 01 Nov 2023 15:53
 Operator : SY/MD
 Sample : VIBLK564
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK564

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 11/02/2023
 Supervised By :Mahesh Dadoda 11/02/2023

Quant Time: Nov 02 03:37:06 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Nov 02 03:33:34 2023
 Response via : Initial Calibration

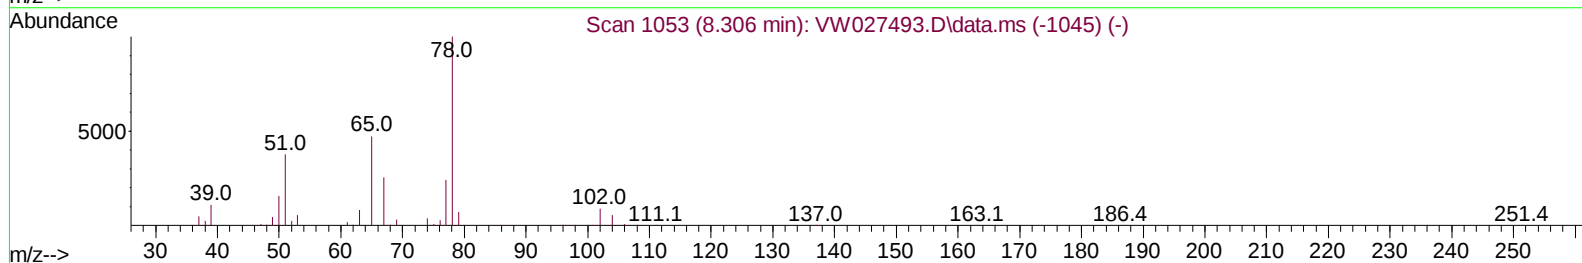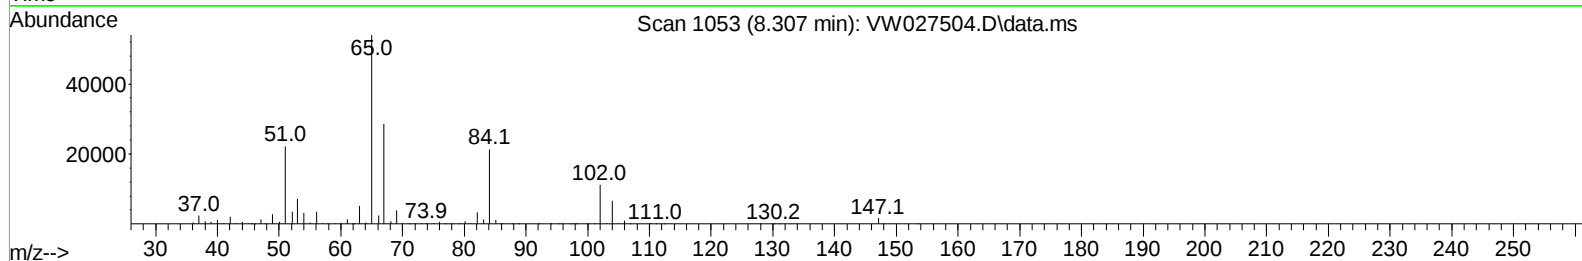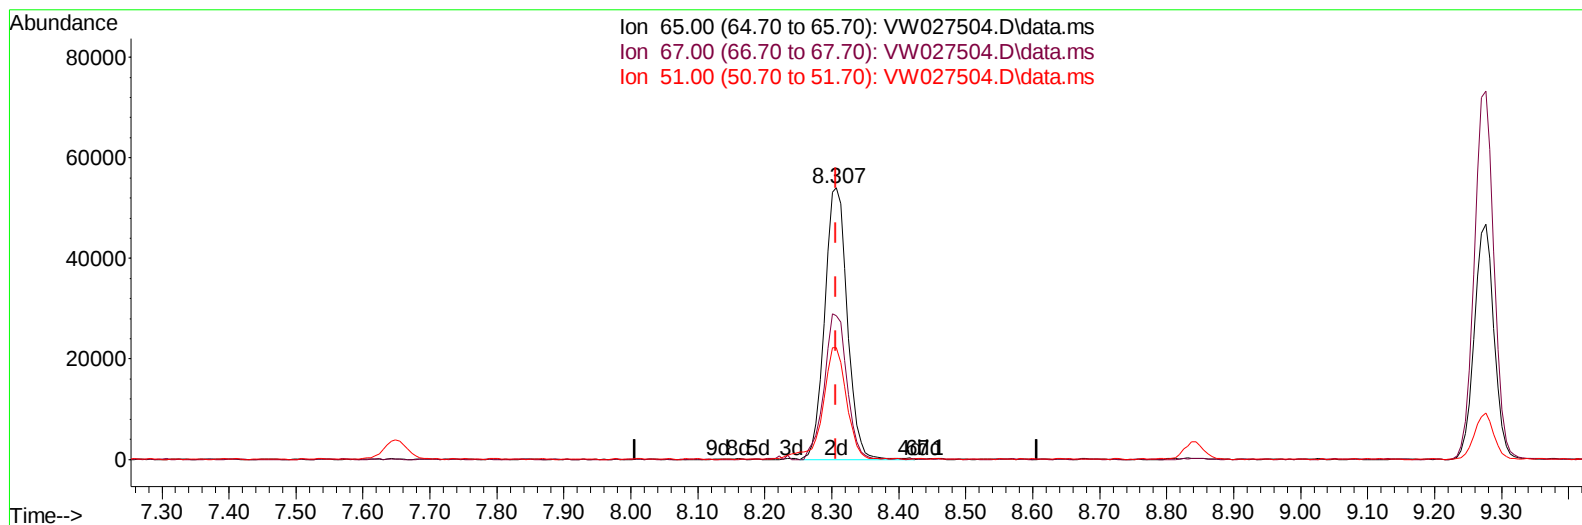

TIC: VW027504.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.000) 23.57 ug/L m

response 126107

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.00	0.06#
51.00	99.60	0.10#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw110123\
 Data File : VW027504.D
 Acq On : 01 Nov 2023 15:53
 Operator : SY/MD
 Sample : VIBLK564
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK564

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 11/02/2023
 Supervised By :Mahesh Dadoda 11/02/2023

Quant Time: Nov 02 03:37:06 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Nov 02 03:33:34 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		334190	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		310395	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		152820	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		105149	20.616	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	82.480%	
7) Chloroethane-d5	2.899	69		86077	23.505	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	94.000%	
11) 1,1-Dichloroethene-d2	4.027	65		52724	20.631	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	82.520%	
21) 2-Butanone-d5	7.081	46		86146	50.817	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	101.640%	
24) Chloroform-d	7.648	84		224087	22.498	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	90.000%	
26) 1,2-Dichloroethane-d4	8.307	65		126107m	23.569	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	94.280%	
32) Benzene-d6	8.276	84		480147	22.864	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	91.440%	
36) 1,2-Dichloropropane-d6	9.276	67		149995	23.384	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	93.520%	
41) Toluene-d8	10.325	98		404523	21.242	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	84.960%	
43) trans-1,3-Dichloroprop...	10.575	79		52740	18.033	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	72.120%	
47) 2-Hexanone-d5	10.922	63		62017	46.731	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	93.460%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		119004	24.867	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	99.480%	
66) 1,2-Dichlorobenzene-d4	13.849	152		119607	21.598	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	86.400%	
Target Compounds							
16) Methylene chloride	4.923	84		10467	1.711	ug/L	86
70) 1,2,4-trichlorobenzene	15.129	180		7781	1.447	ug/L	98
72) 1,2,3-Trichlorobenzene	15.543	180		9381	2.121	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110123\
Data File : VW027504.D
Acq On : 01 Nov 2023 15:53
Operator : SY/MD
Sample : VIBLK564
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK564

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 11/02/2023
Supervised By :Mahesh Dadoda 11/02/2023

Quant Time: Nov 02 03:37:06 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101123SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Nov 02 03:33:34 2023
Response via : Initial Calibration

