

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110123\
 Data File : VW027511.D
 Acq On : 01 Nov 2023 18:40
 Operator : SY/MD
 Sample : 05174-15
 Misc : 6.17g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AN7

Quant Time: Nov 02 03:38:29 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Nov 02 03:33:34 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	499715	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	476016	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	247630	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	91819	12.040	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	48.160%
7) Chloroethane-d5	2.893	69	83582	15.263	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	61.040%
11) 1,1-Dichloroethene-d2	4.015	65	53161	13.911	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	55.640%
21) 2-Butanone-d5	7.075	46	108596	42.841	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.680%
24) Chloroform-d	7.648	84	279697	18.779	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	75.120%
26) 1,2-Dichloroethane-d4	8.307	65	156121	19.513	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	78.040%
32) Benzene-d6	8.276	84	543092	16.863	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	67.440%
36) 1,2-Dichloropropane-d6	9.270	67	186867	18.997	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	76.000%
41) Toluene-d8	10.319	98	465286	15.932	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	63.720%
43) trans-1,3-Dichloroprop...	10.575	79	65453	14.594	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	58.360%
47) 2-Hexanone-d5	10.922	63	82201	40.389	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	80.780%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	162560	22.150	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	88.600%
66) 1,2-Dichlorobenzene-d4	13.849	152	157730	17.577	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	70.320%#
Target Compounds						
16) Methylene chloride	4.923	84	24626	2.692	ug/L	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110123\
Data File : VW027511.D
Acq On : 01 Nov 2023 18:40
Operator : SY/MD
Sample : 05174-15
Misc : 6.17g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AN7


Quant Time: Nov 02 03:38:29 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101123SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Nov 02 03:33:34 2023
Response via : Initial Calibration

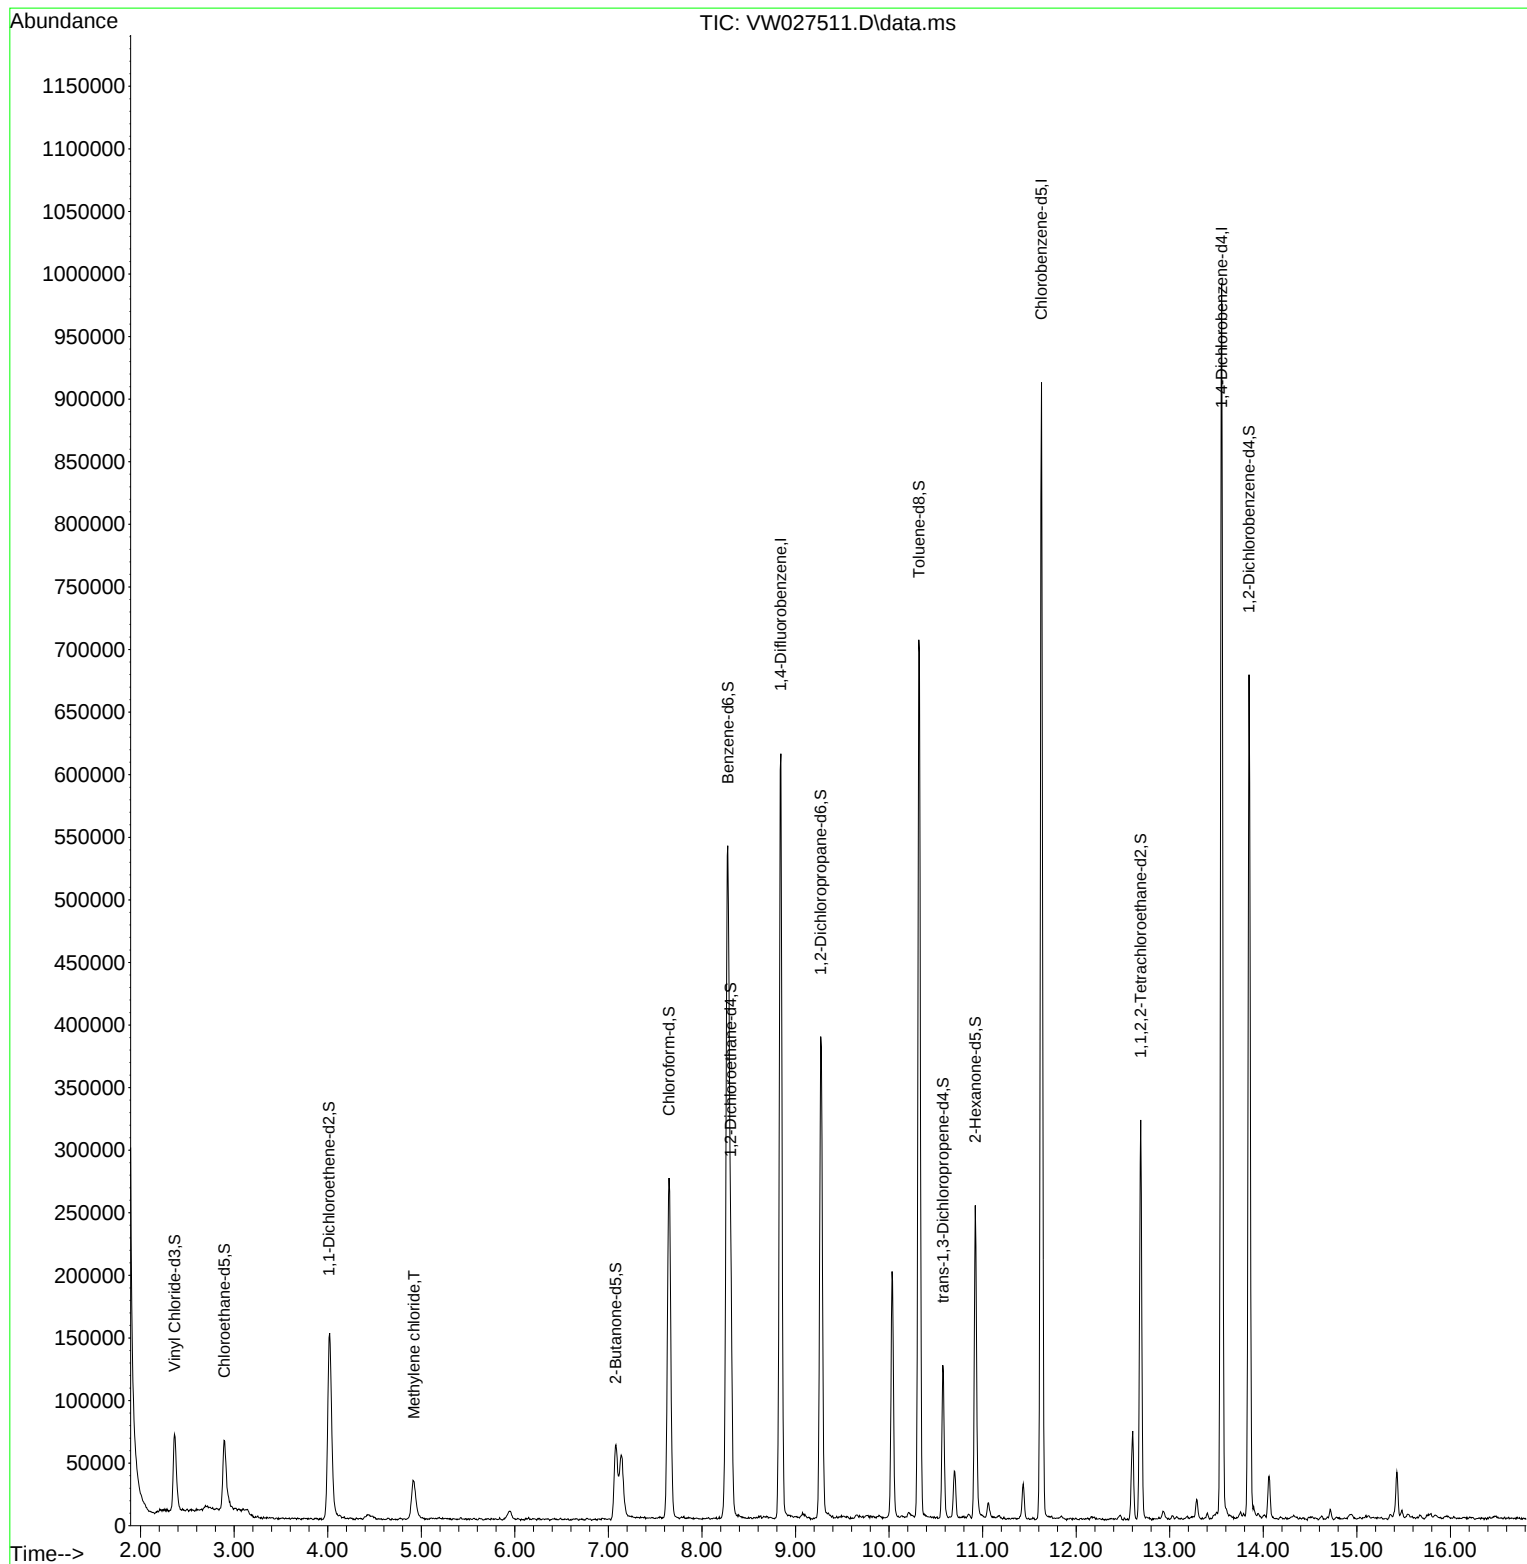

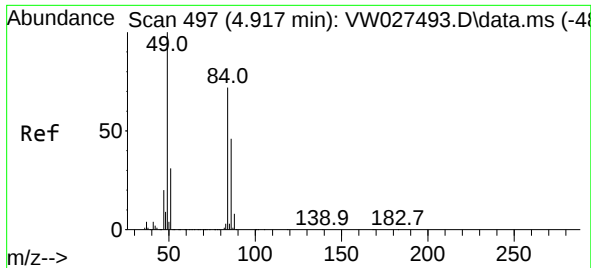

#16
Methylene chloride
Concen: 2.692 ug/L
RT: 4.923 min Scan# 49
Delta R.T. 0.006 min
Lab File: VW027511.D
Acq: 01 Nov 2023 18:40

Instrument :
MSVOA_W
ClientSampleId :
C0AN7

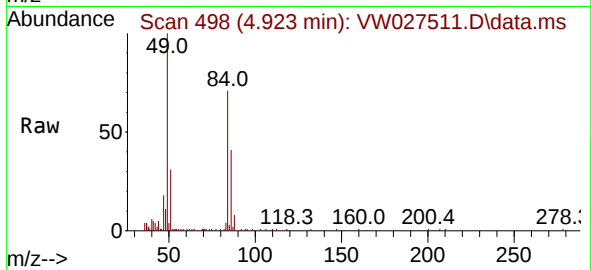

Tgt Ion: 84 Resp: 24626

Ion	Ratio	Lower	Upper
84	100		
86	57.6	41.3	76.7
49	141.6	92.8	172.4

