




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110124\
 Data File : VW030877.D
 Acq On : 01 Nov 2024 11:13
 Operator : SY/MD
 Sample : P4603-01
 Misc : 5.64g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4EC8

Manual IntegrationsAPPROVED

Quant Time: Nov 04 00:54:01 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Nov 01 03:09:59 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 11/04/2024
 Supervised By :Mahesh Dadoda 11/05/2024

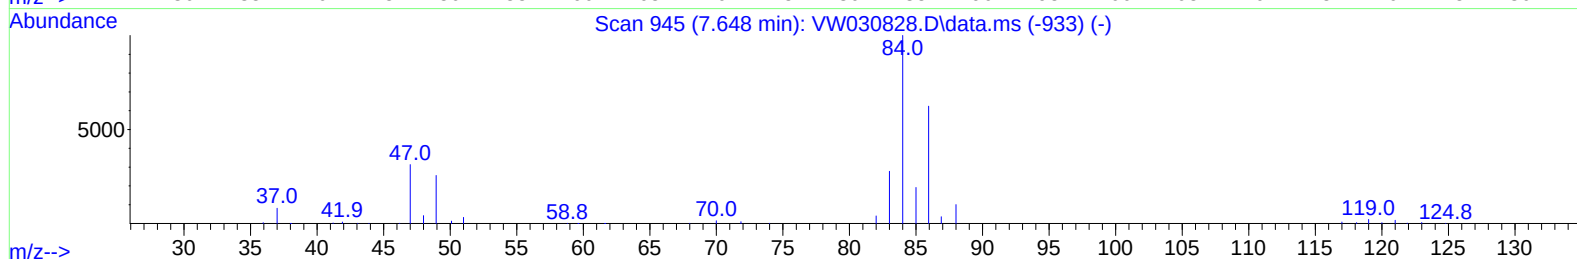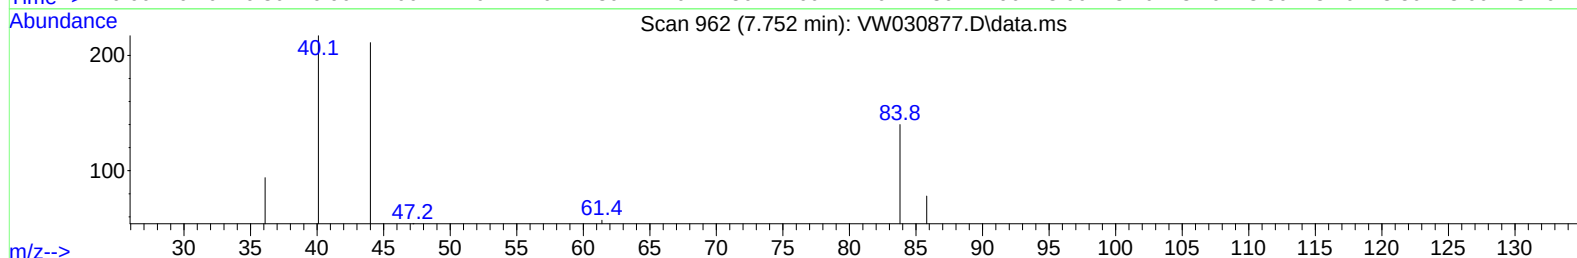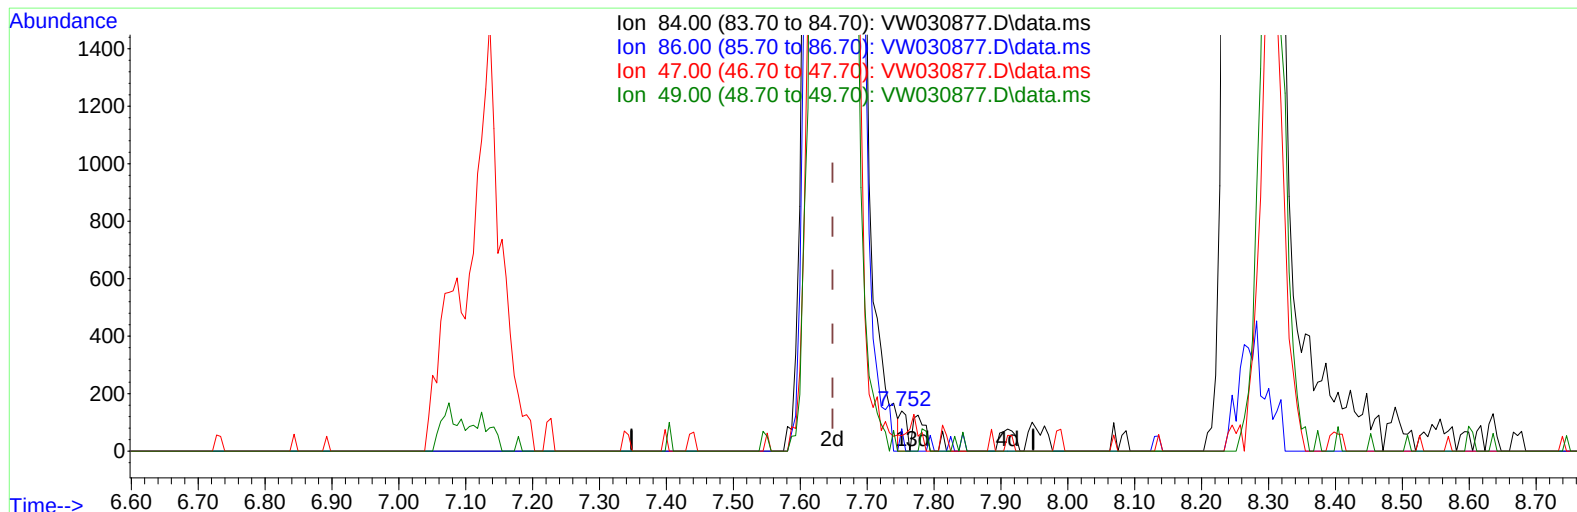

TIC: VW030877.D\data.ms

(24) Chloroform-d (S)

7.752min (+ 0.103) 0.01 ug/L

response 97

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.10	61.86
47.00	48.90	46.39
49.00	28.60	26.80




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110124\
Data File : VW030877.D
Acq On : 01 Nov 2024 11:13
Operator : SY/MD
Sample : P4603-01
Misc : 5.64g/10mL/MSVOA_W/SOIL/B
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4EC8

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 11/04/2024
Supervised By :Mahesh Dadoda 11/05/2024

Quant Time: Nov 04 00:54:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Nov 01 03:09:59 2024
Response via : Initial Calibration

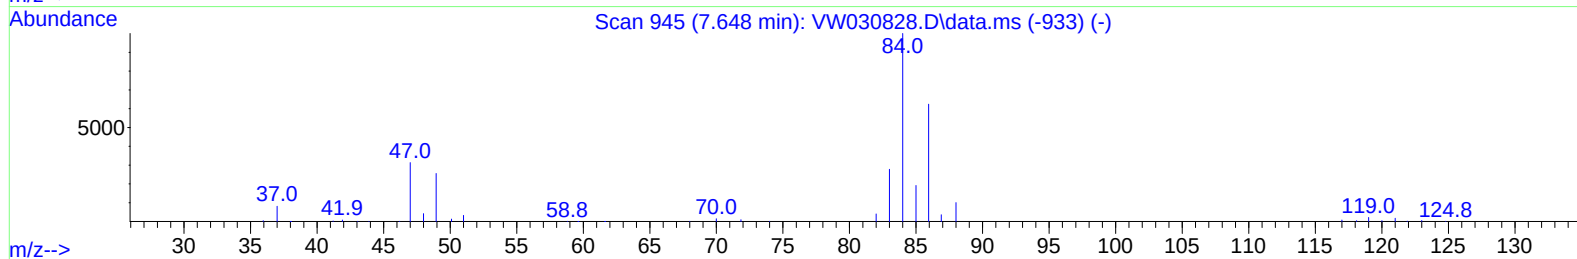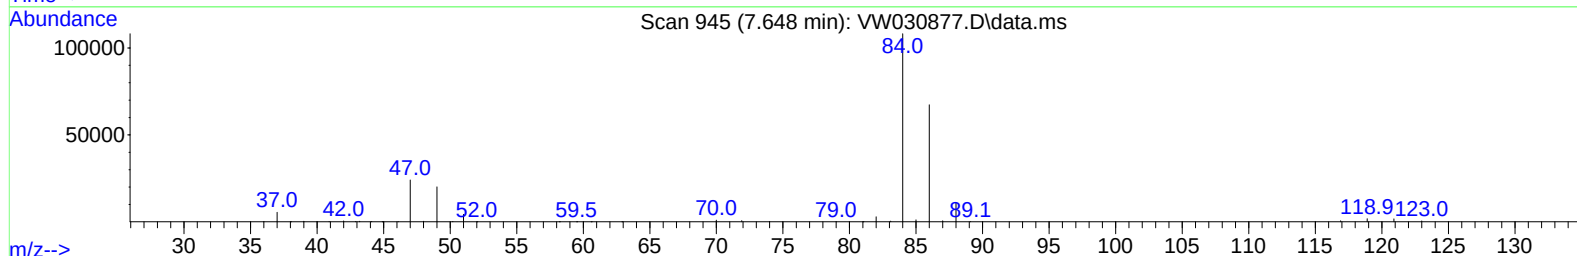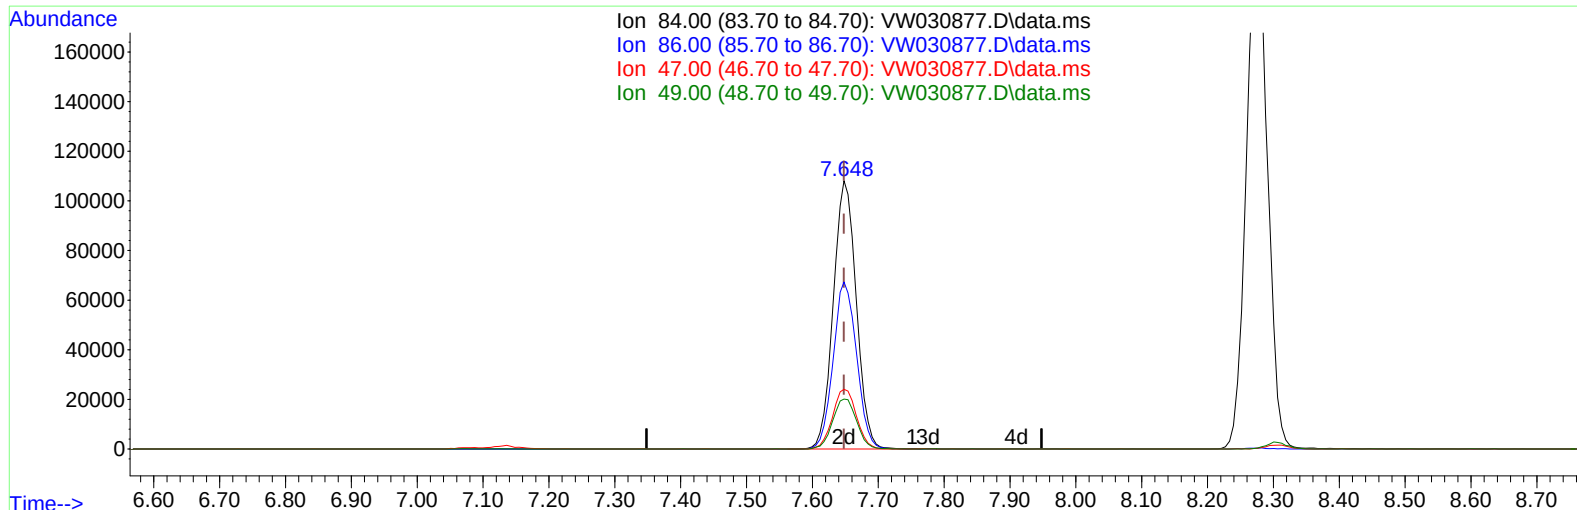

TIC: VW030877.D\data.ms

(24) Chloroform-d (S)

7.648min (-0.000) 23.49 ug/L m

response 262351

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.10	0.02#
47.00	48.90	0.02#
49.00	28.60	0.01#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110124\
 Data File : VW030877.D
 Acq On : 01 Nov 2024 11:13
 Operator : SY/MD
 Sample : P4603-01
 Misc : 5.64g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4EC8

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 11/04/2024
 Supervised By :Mahesh Dadoda 11/05/2024

Quant Time: Nov 04 00:54:01 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Nov 01 03:09:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	390587	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	361085	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	155682	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	115442	18.803	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	75.200%		
7) Chloroethane-d5	2.899	69	101955	21.939	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	87.760%		
11) 1,1-Dichloroethene-d2	4.021	65	46290	18.128	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	72.520%		
21) 2-Butanone-d5	7.075	46	59282	53.655	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	107.320%		
24) Chloroform-d	7.648	84	262351m	23.487	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	93.960%		
26) 1,2-Dichloroethane-d4	8.306	65	145720	25.088	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	100.360%		
32) Benzene-d6	8.276	84	466368	22.253	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	89.000%		
36) 1,2-Dichloropropane-d6	9.276	67	147976	24.057	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	96.240%		
41) Toluene-d8	10.324	98	412259	21.549	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	86.200%		
43) trans-1,3-Dichloroprop...	10.574	79	58410	22.677	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	90.720%		
47) 2-Hexanone-d5	10.922	63	45842	57.862	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	115.720%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	121298	26.851	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	107.400%		
66) 1,2-Dichlorobenzene-d4	13.848	152	141961	26.950	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	107.800%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110124\
Data File : VW030877.D
Acq On : 01 Nov 2024 11:13
Operator : SY/MD
Sample : P4603-01
Misc : 5.64g/10mL/MSVOA_W/SOIL/B
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4EC8

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 11/04/2024
Supervised By :Mahesh Dadoda 11/05/2024

Quant Time: Nov 04 00:54:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Nov 01 03:09:59 2024
Response via : Initial Calibration

