

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110124\
 Data File : VW030884.D
 Acq On : 01 Nov 2024 14:35
 Operator : SY/MD
 Sample : P4586-01
 Misc : 5.39g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4EE1

Quant Time: Nov 04 00:54:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Nov 01 03:09:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	377582	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	361640	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	158309	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	105043	17.699	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.800%
7) Chloroethane-d5	2.899	69	91215	20.304	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.200%
11) 1,1-Dichloroethene-d2	4.015	65	45454	18.413	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	73.640%
21) 2-Butanone-d5	7.075	46	48217	45.144	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.280%
24) Chloroform-d	7.648	84	227601	21.078	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	84.320%
26) 1,2-Dichloroethane-d4	8.301	65	122232	21.769	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	87.080%
32) Benzene-d6	8.276	84	403073	19.204	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	76.800%
36) 1,2-Dichloropropane-d6	9.270	67	126873	20.594	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	82.360%
41) Toluene-d8	10.319	98	351271	18.333	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	73.320%
43) trans-1,3-Dichloroprop...	10.575	79	47369	18.362	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	73.440%
47) 2-Hexanone-d5	10.922	63	36504	46.005	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.000%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	98542	21.780	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	87.120%
66) 1,2-Dichlorobenzene-d4	13.849	152	123091	22.980	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.920%
Target Compounds					Qvalue	
72) 1,2,3-Trichlorobenzene	15.549	180	1688	0.344	ug/L #	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110124\
Data File : VW030884.D
Acq On : 01 Nov 2024 14:35
Operator : SY/MD
Sample : P4586-01
Misc : 5.39g/10mL/MSVOA_W/SOIL/A
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4EE1


Quant Time: Nov 04 00:54:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Nov 01 03:09:59 2024
Response via : Initial Calibration

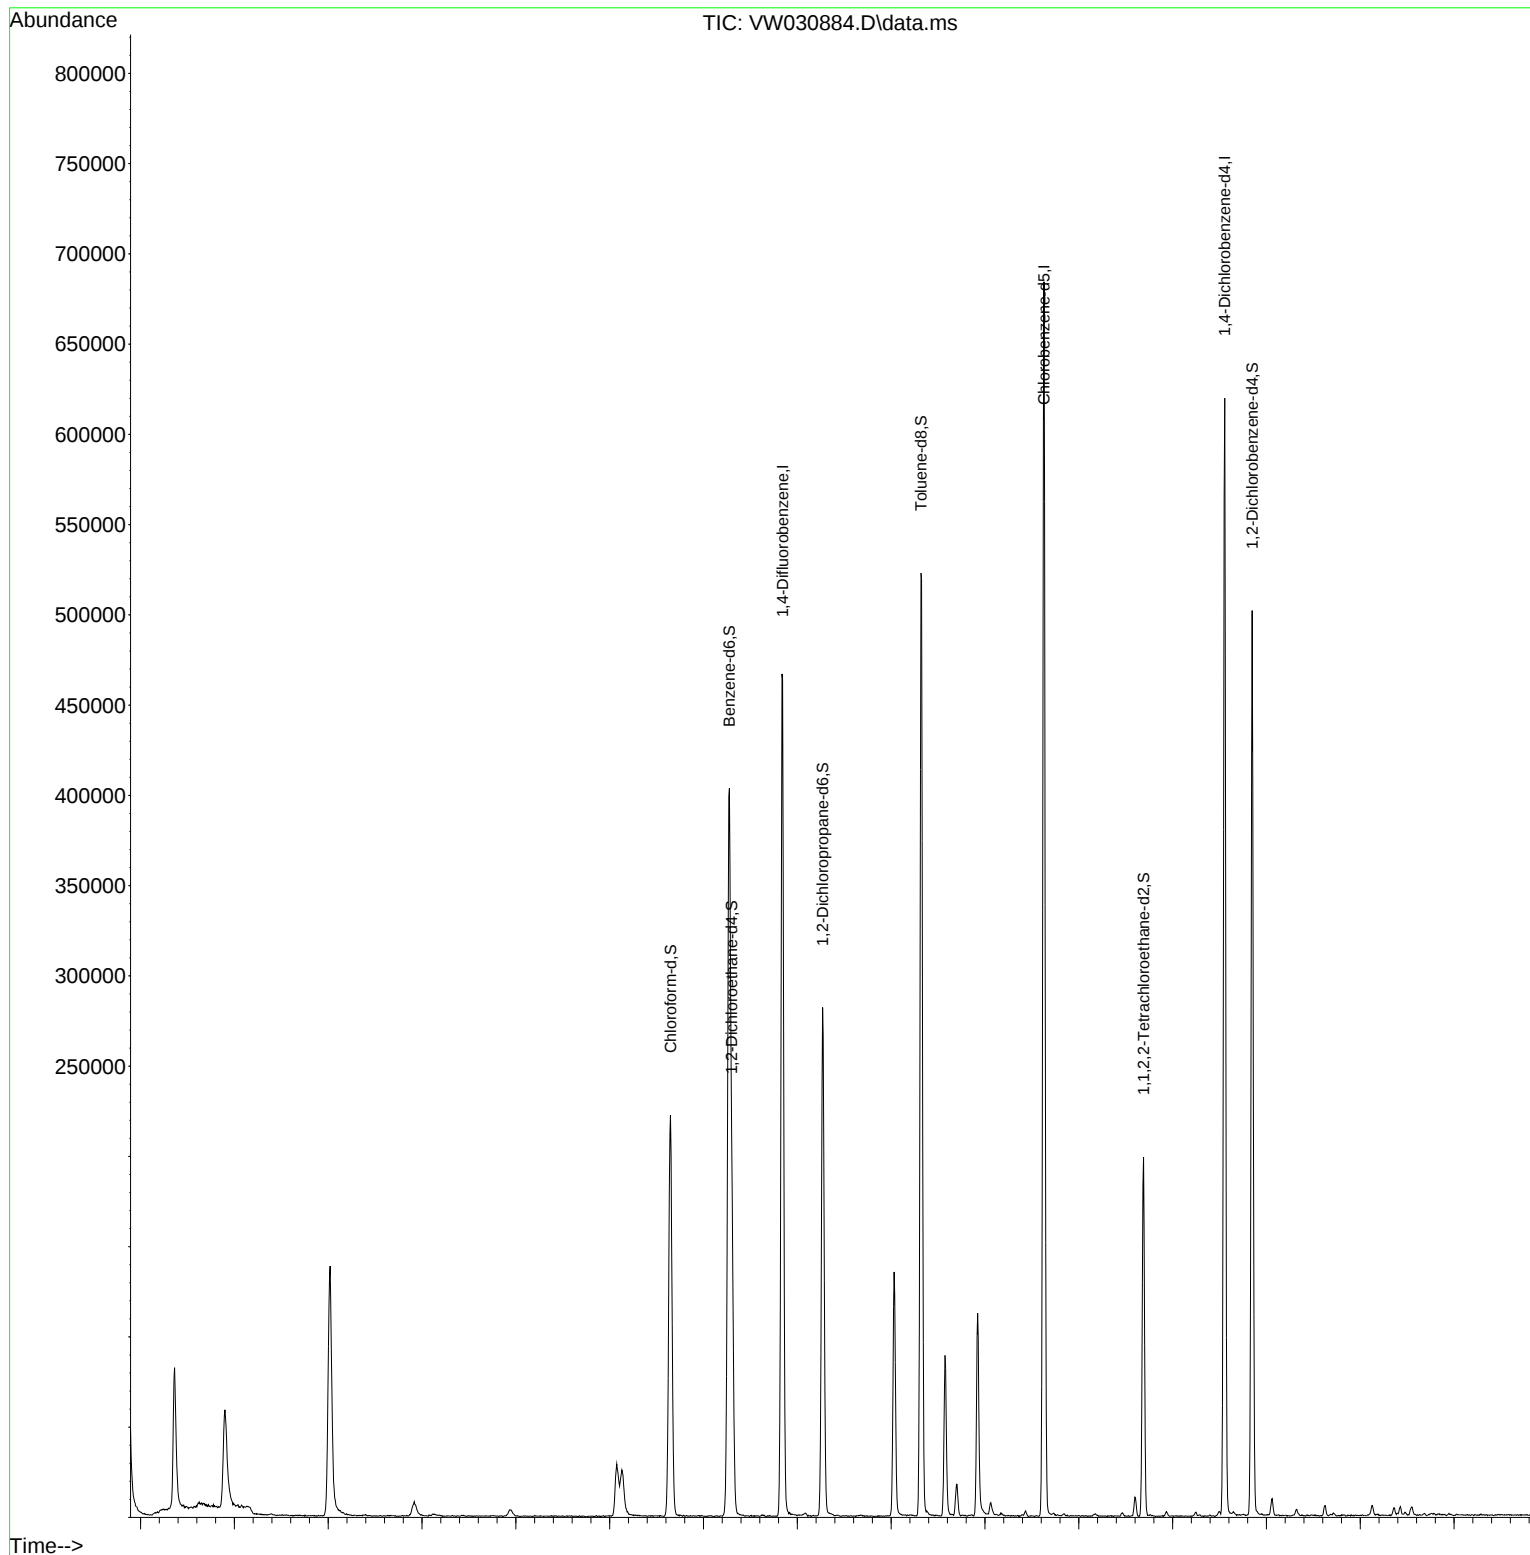

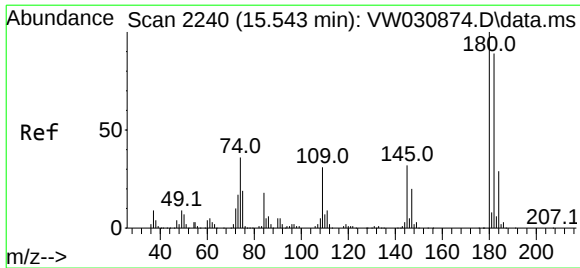

#72
1,2,3-Trichlorobenzene
Concen: 0.344 ug/L
RT: 15.549 min Scan# 2241
Delta R.T. 0.000 min
Lab File: VW030884.D
Acq: 01 Nov 2024 14:35

Instrument :
MSVOA_W
ClientSampleId :
A4EE1

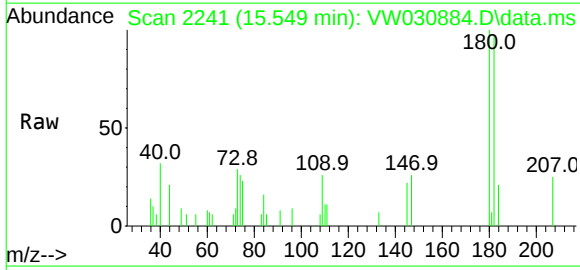

Tgt Ion:	180	Resp:	1688
Ion	Ratio	Lower	Upper
180	100		
182	87.7	76.2	114.4
145	21.6	27.4	41.2

