

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110222\
 Data File : VW025004.D
 Acq On : 02 Nov 2022 13:53
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK575

Quant Time: Nov 03 06:29:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 27 23:51:01 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	283210	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	257885	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	122439	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	62900	19.787	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.160%
7) Chloroethane-d5	2.891	69	35724	19.184	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.720%
11) 1,1-Dichloroethene-d2	4.019	63	136530	17.242	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.960%
21) 2-Butanone-d5	7.080	46	40999	38.215	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	76.420%
24) Chloroform-d	7.653	84	201820	23.481	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.920%
26) 1,2-Dichloroethane-d4	8.305	65	111993	23.278	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	93.120%
32) Benzene-d6	8.275	84	392454	23.743	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.960%
36) 1,2-Dichloropropane-d6	9.274	67	110265	22.767	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.080%
41) Toluene-d8	10.323	98	367939	23.910	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	95.640%
43) trans-1,3-Dichloroprop...	10.579	79	48351	22.514	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	90.040%
47) 2-Hexanone-d5	10.927	63	33342	39.853	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	79.700%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	80852	20.907	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	83.640%
66) 1,2-Dichlorobenzene-d4	13.847	152	112381	23.884	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.520%
Target Compounds						Qvalue
37) 1,2-Dichloropropane	9.274	63	14397	3.820	ug/L	# 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110222\
Data File : VW025004.D
Acq On : 02 Nov 2022 13:53
Operator : SY/VA
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK575

Quant Time: Nov 03 06:29:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 27 23:51:01 2022
Response via : Initial Calibration

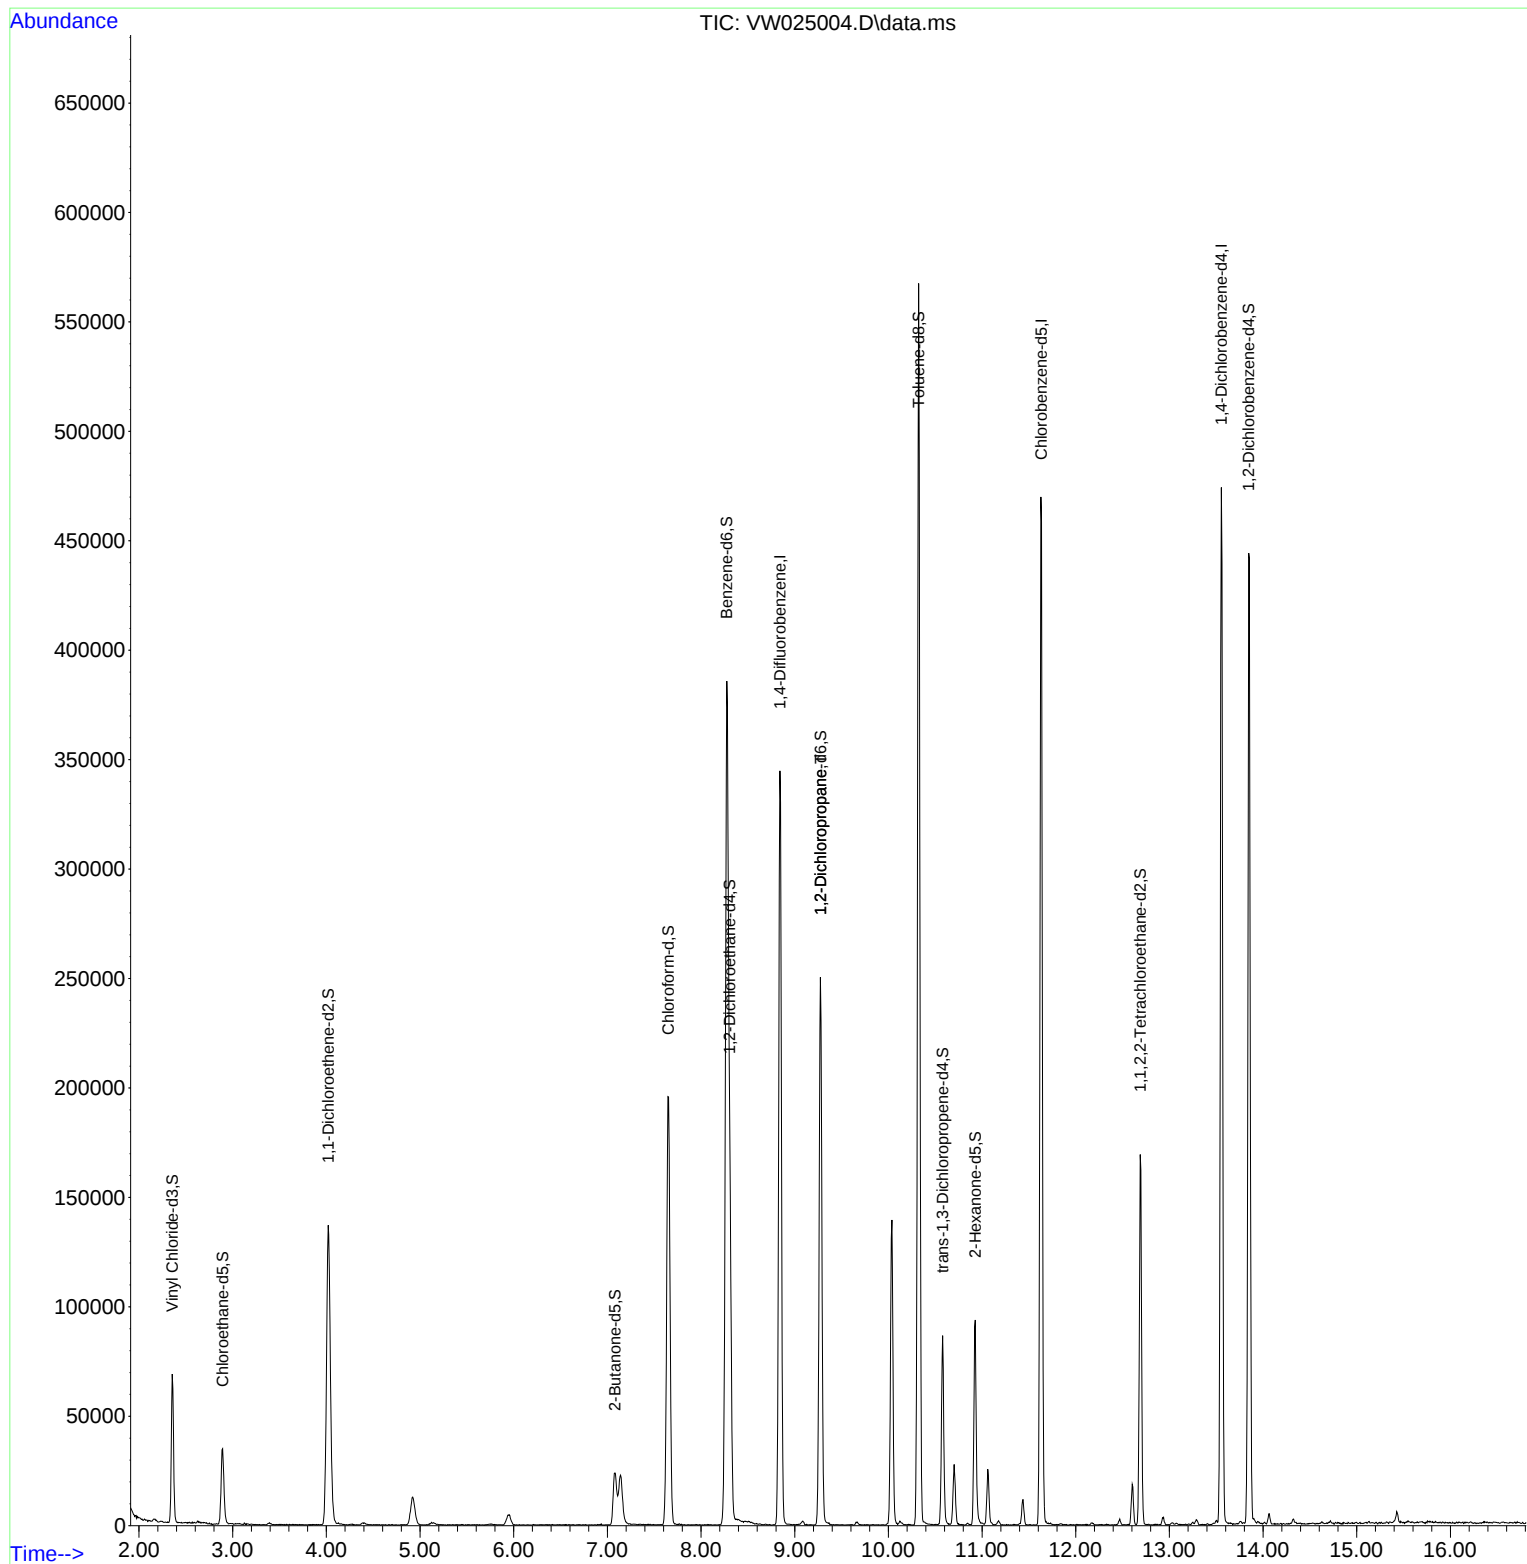

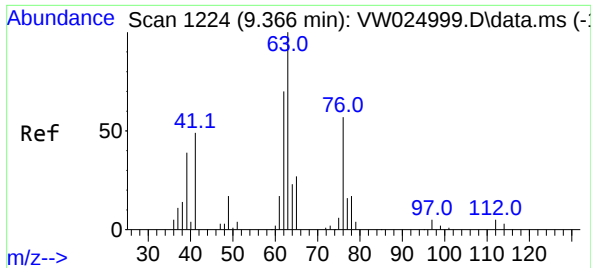

#37
 1,2-Dichloropropane
 Concen: 3.820 ug/L
 RT: 9.274 min Scan# 11
 Delta R.T. -0.091 min
 Lab File: VW025004.D
 Acq: 02 Nov 2022 13:53

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK575

Tgt Ion: 63 Resp: 14397
 Ion Ratio Lower Upper
 63 100
 112 0.0 3.6 5.4#

