

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110222\
 Data File : VW025008.D
 Acq On : 02 Nov 2022 15:29
 Operator : SY/VA
 Sample : VIBLK577
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK577

Quant Time: Nov 03 06:30:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 27 23:51:01 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	259561	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	248262	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	119495	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	52403	17.987	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	71.960%
7) Chloroethane-d5	2.891	69	30450	17.842	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	71.360%
11) 1,1-Dichloroethene-d2	4.019	63	107837	14.859	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	59.440%
21) 2-Butanone-d5	7.080	46	39486	40.158	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	80.320%
24) Chloroform-d	7.647	84	166695	21.162	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	84.640%
26) 1,2-Dichloroethane-d4	8.305	65	98263	22.285	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	89.120%
32) Benzene-d6	8.275	84	323702	20.343	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	81.360%
36) 1,2-Dichloropropane-d6	9.274	67	92811	19.906	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	79.640%
41) Toluene-d8	10.323	98	296272	19.999	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	80.000%
43) trans-1,3-Dichloroprop...	10.579	79	41531	20.088	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	80.360%
47) 2-Hexanone-d5	10.927	63	32151	39.919	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	79.840%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	73586	19.766	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	79.080%
66) 1,2-Dichlorobenzene-d4	13.847	152	95803	20.862	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	83.440%
Target Compounds						Qvalue
16) Methylene chloride	4.915	84	23990	5.206	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110222\
Data File : VW025008.D
Acq On : 02 Nov 2022 15:29
Operator : SY/VA
Sample : VIBLK577
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK577

Quant Time: Nov 03 06:30:31 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 27 23:51:01 2022
Response via : Initial Calibration

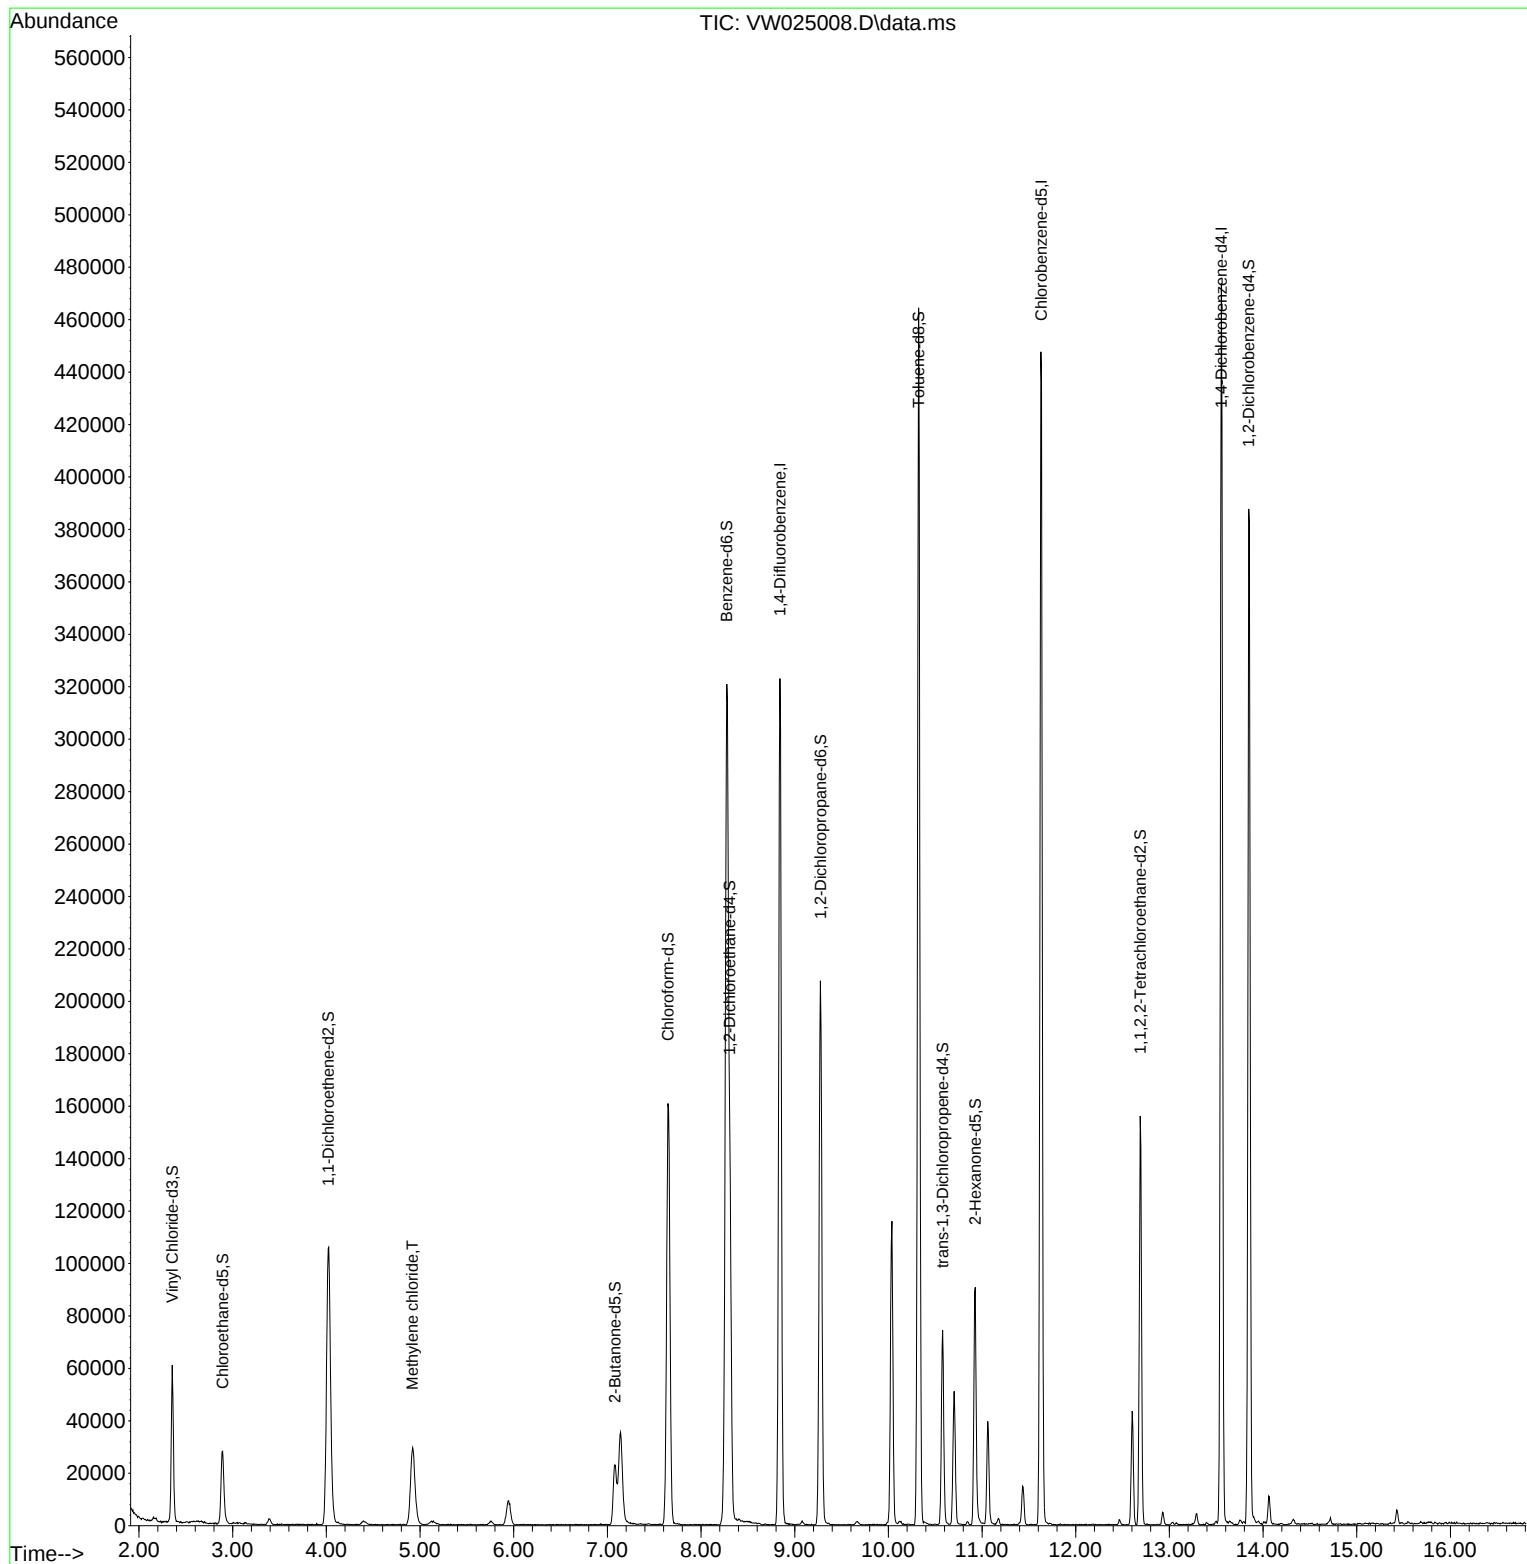

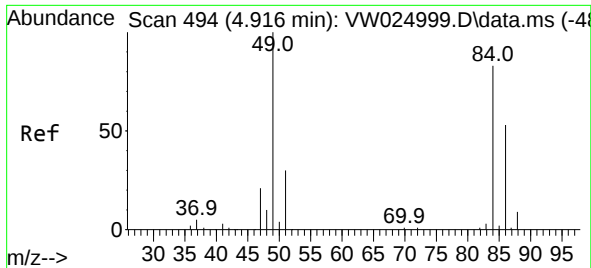

#16

Methylene chloride

Concen: 5.206 ug/L

RT: 4.915 min Scan# 49

Delta R.T. -0.006 min

Lab File: VW025008.D


Acq: 02 Nov 2022 15:29

Instrument :

MSVOA_W

ClientSampleId :

VIBLK577

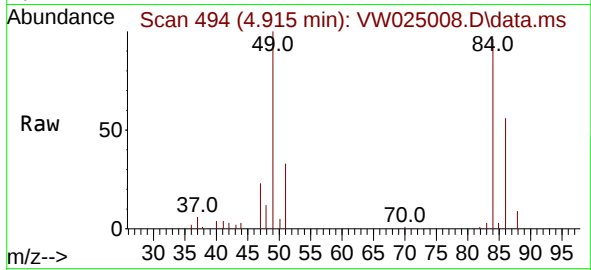

Tgt Ion: 84 Resp: 23990

Ion Ratio Lower Upper

84 100

86 57.7 42.6 79.0

49 103.9 81.9 152.1

