

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110222\
 Data File : VW025011.D
 Acq On : 02 Nov 2022 16:41
 Operator : SY/VA
 Sample : VIBLK578
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK578

Quant Time: Nov 03 06:30:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 27 23:51:01 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	270807	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	248522	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	117616	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	65590	21.578	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	86.320%
7) Chloroethane-d5	2.885	69	39383	22.118	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.480%
11) 1,1-Dichloroethene-d2	4.019	63	138000	18.226	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	72.920%
21) 2-Butanone-d5	7.080	46	46326	45.158	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.320%
24) Chloroform-d	7.653	84	207812	25.286	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	101.160%
26) 1,2-Dichloroethane-d4	8.305	65	117121	25.459	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	101.840%
32) Benzene-d6	8.275	84	404602	25.400	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	101.600%
36) 1,2-Dichloropropane-d6	9.274	67	113745	24.370	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.480%
41) Toluene-d8	10.323	98	374029	25.221	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	100.880%
43) trans-1,3-Dichloroprop...	10.579	79	49004	23.678	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	94.720%
47) 2-Hexanone-d5	10.921	63	37908	47.017	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.040%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	88737	23.811	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.240%
66) 1,2-Dichlorobenzene-d4	13.847	152	116248	25.719	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.880%
Target Compounds						Qvalue
16) Methylene chloride	4.915	84	26836	5.581	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110222\
Data File : VW025011.D
Acq On : 02 Nov 2022 16:41
Operator : SY/VA
Sample : VIBLK578
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK578

Quant Time: Nov 03 06:30:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 27 23:51:01 2022
Response via : Initial Calibration

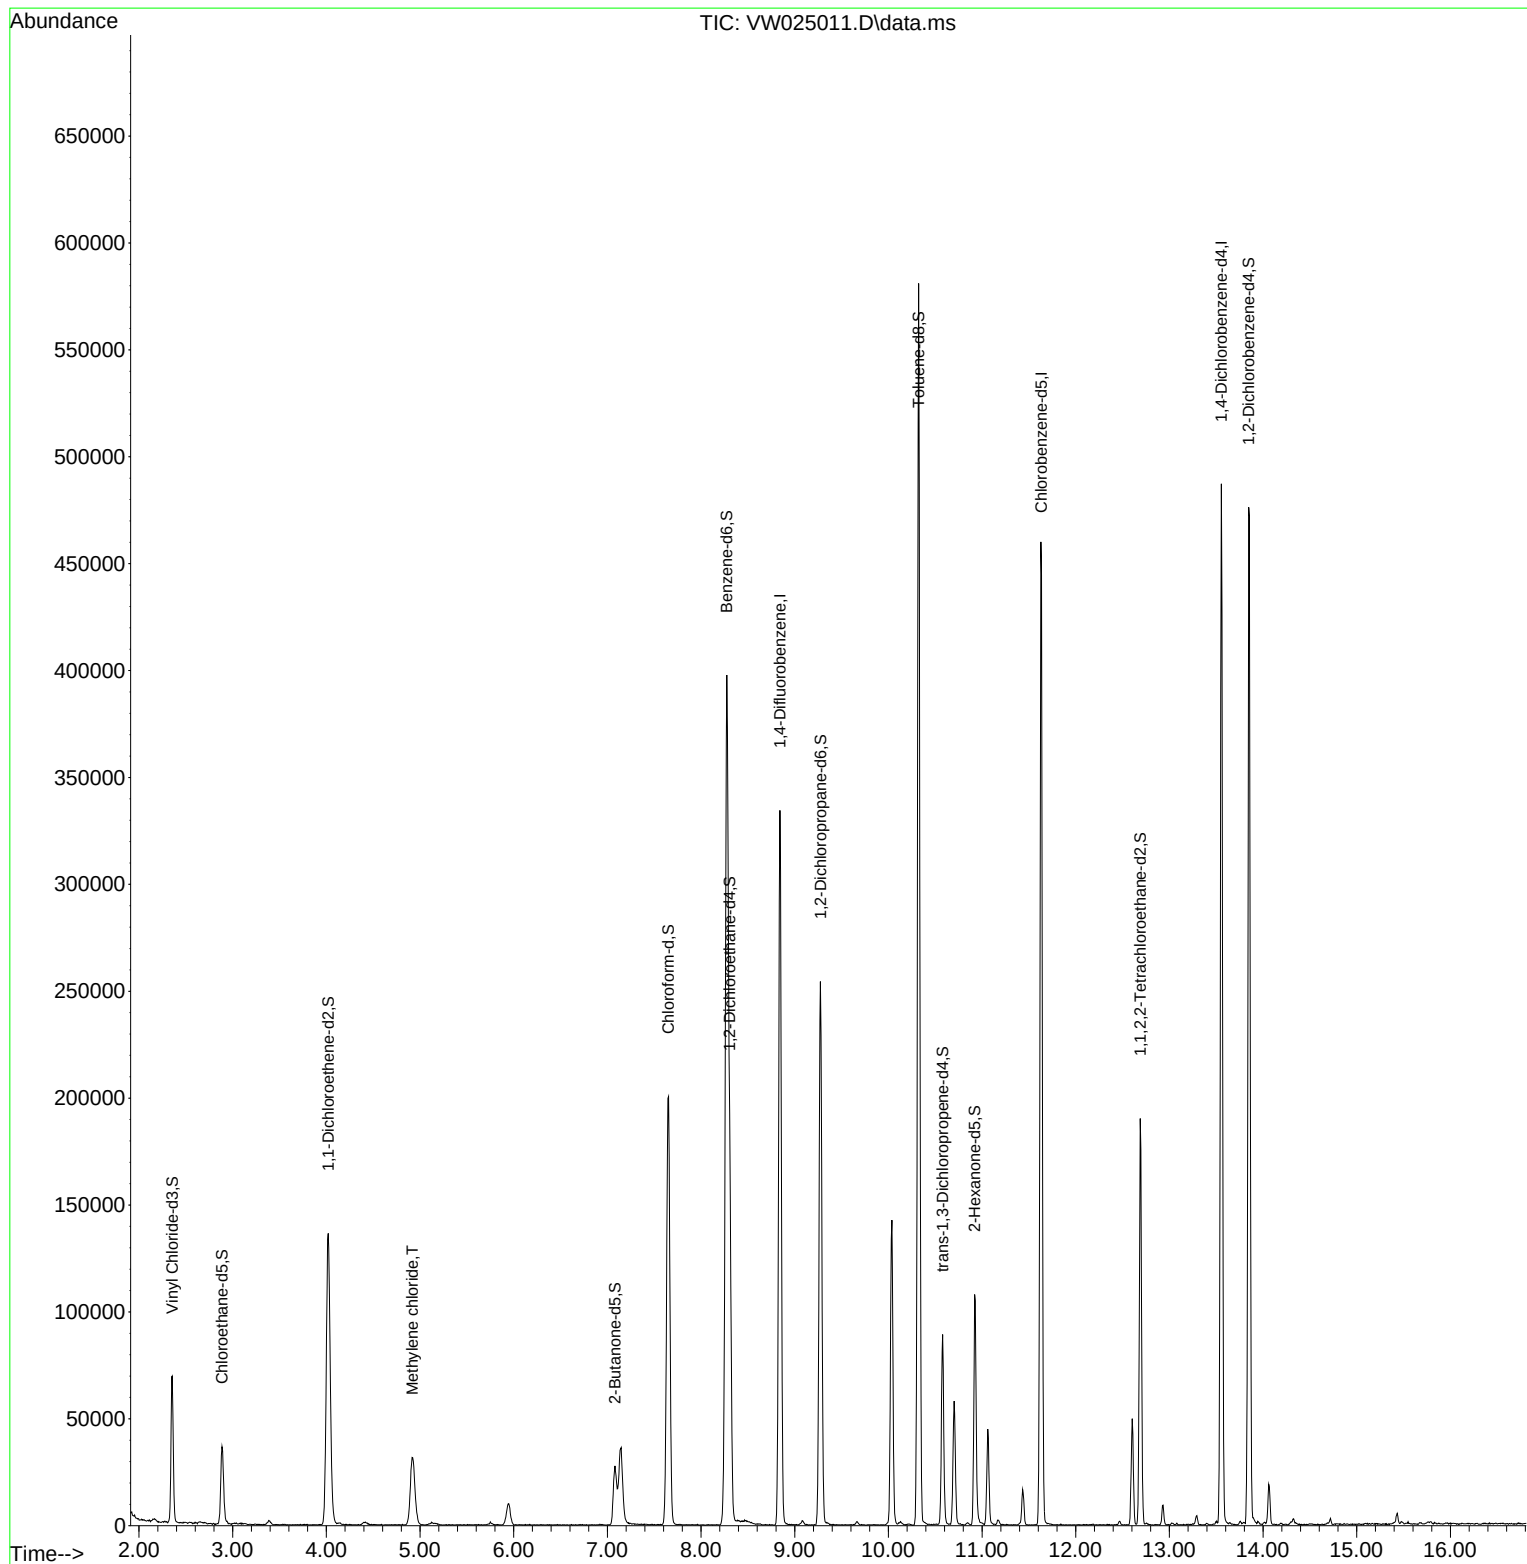

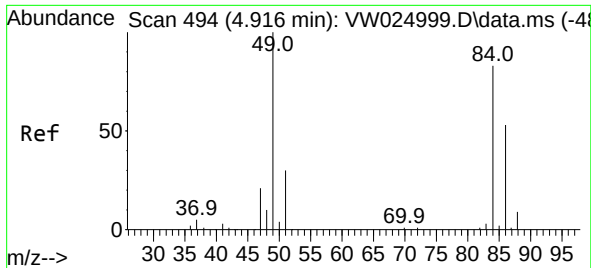

#16
Methylene chloride
Concen: 5.581 ug/L
RT: 4.915 min Scan# 49
Delta R.T. -0.006 min
Lab File: VW025011.D
Acq: 02 Nov 2022 16:41

Instrument :
MSVOA_W
ClientSampleId :
VIBLK578

Tgt Ion: 84 Resp: 26836
Ion Ratio Lower Upper
84 100
86 66.0 42.6 79.0
49 120.2 81.9 152.1

