
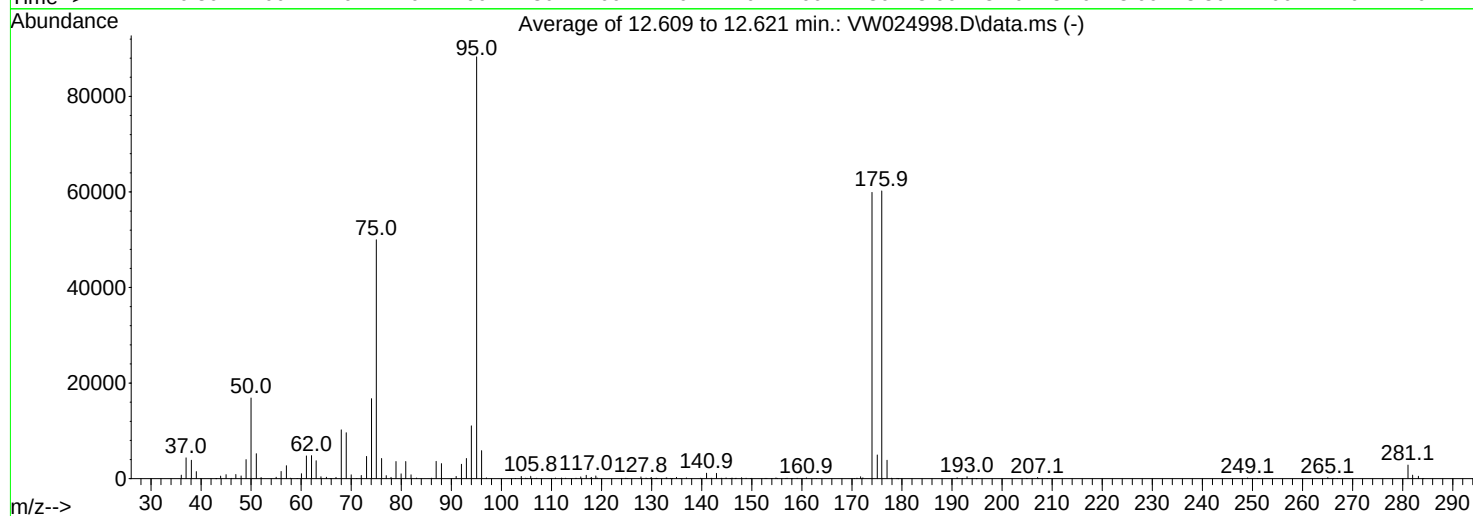


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110222\
Data File : VW024998.D
Acq On : 02 Nov 2022 09:22
Operator : SY/VA
Sample : BFB449
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB449

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
Title : SFAM01.0
Last Update : Thu Oct 27 23:51:01 2022

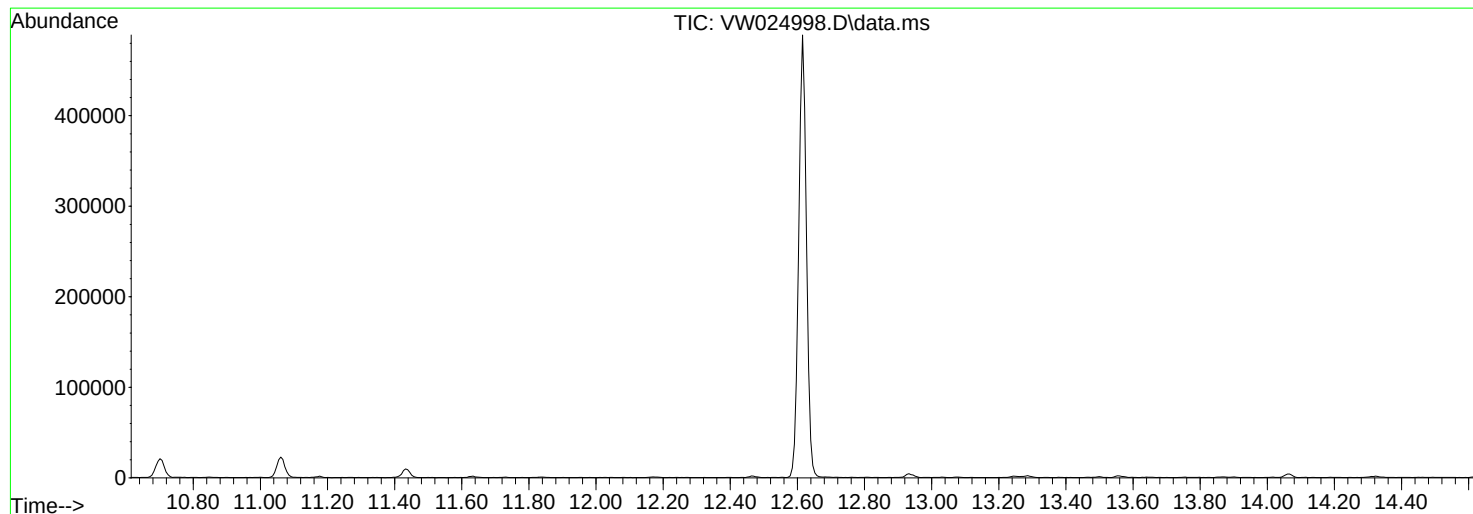

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	16888	PASS
75	95	30	80	56.6	49989	PASS
95	95	100	100	100.0	88275	PASS
96	95	5	9	6.7	5876	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	67.9	59920	PASS
175	174	5	9	8.3	4961	PASS
176	174	95	105	100.5	60205	PASS
177	176	5	10	6.4	3868	PASS

m/z	Abundance
39.90	223.0
43.00	64.0
43.80	139.0

Instrument :
MSVOA_W
ClientSampleId :
BFB449

m/z	Abundance
36.10	727.0
37.00	4648.0
38.00	3827.0
39.10	1313.0
40.10	334.0
42.90	103.0
44.00	681.0
45.00	953.0
46.90	864.0
48.10	542.0
49.00	3792.0
50.00	15936.0
51.00	5542.0
52.10	200.0
55.00	324.0
56.00	1567.0
57.10	2563.0
57.80	148.0
59.20	108.0
60.00	963.0
61.10	4904.0
62.00	4835.0
63.00	3571.0
64.00	436.0
65.10	310.0
66.90	333.0
68.00	9761.0
69.00	9658.0
70.00	897.0
71.10	63.0
72.00	763.0
73.00	4647.0
74.00	15896.0
75.00	48128.0
76.00	4183.0
77.10	586.0
78.90	2985.0
80.00	1040.0
80.90	3203.0
81.90	841.0
83.10	118.0
86.00	86.0
87.00	3451.0
88.00	2961.0
90.90	461.0
92.00	2869.0
93.00	3940.0
94.00	11112.0
95.00	83944.0
96.00	5385.0
96.90	121.0
104.00	454.0
105.10	159.0
105.80	632.0
107.00	110.0
109.90	69.0
110.80	106.0
112.00	149.0
112.90	142.0
114.90	74.0
115.80	339.0
117.00	730.0
117.80	355.0
118.90	586.0
124.00	75.0
124.90	158.0
127.90	349.0
128.90	136.0
129.80	442.0
131.00	104.0
132.90	500.0
133.80	100.0
135.00	298.0
135.70	77.0
136.90	180.0
139.80	55.0
141.00	933.0
142.00	119.0
142.90	1107.0
144.00	87.0
144.90	134.0
146.00	153.0
146.70	89.0
147.90	267.0
148.80	120.0
149.80	103.0
153.00	87.0
154.80	290.0
157.00	99.0
159.00	112.0
160.90	126.0
162.90	73.0

Instrument :
MSVOA_W
ClientSampleId :
BFB449

170.40	62.0
171.00	149.0
171.70	348.0
174.00	48856.0
175.10	4122.0
175.90	49112.0
177.00	3367.0
177.90	107.0
179.00	169.0
191.00	306.0
192.10	91.0
193.00	532.0
194.00	151.0
194.80	54.0
204.90	153.0
207.10	363.0
209.00	96.0
249.10	320.0
251.00	110.0
265.10	423.0
266.20	65.0
266.90	110.0
280.00	145.0
281.00	3878.0
282.00	1148.0
283.20	706.0
284.00	138.0

Instrument :
MSVOA_W
ClientSampleId :
BFB449

m/z	Abundance
36.00	796.0
37.00	4797.0
38.10	4371.0
39.10	1493.0
39.90	231.0
43.00	143.0
43.90	622.0
45.00	986.0
46.10	59.0
47.00	927.0
47.90	797.0
49.00	4772.0
50.00	19568.0
51.00	5690.0
52.00	347.0
55.00	317.0
56.00	1690.0
57.00	3046.0
57.90	137.0
60.10	1286.0
61.00	5430.0
62.00	5310.0
63.00	4071.0
63.90	482.0
65.10	335.0
65.80	51.0
67.00	340.0
68.00	11167.0
69.00	10786.0
70.00	953.0
72.00	773.0
73.10	5023.0
74.00	18960.0
75.00	56688.0
76.10	4646.0
76.90	766.0
78.00	351.0
79.00	4279.0
79.90	943.0
80.90	3889.0
82.00	691.0
83.00	170.0
86.00	90.0
87.00	4102.0
88.00	3683.0
91.00	481.0
92.00	3441.0
93.00	4608.0
94.00	12804.0
95.10	97744.0
96.00	6665.0
97.00	147.0
102.80	119.0
104.00	549.0
104.80	144.0
105.90	558.0
107.10	135.0
109.90	84.0
110.80	140.0
112.10	82.0
112.80	128.0
114.90	128.0
115.80	390.0
116.90	752.0
118.00	477.0
118.90	713.0
124.00	107.0
124.80	127.0
127.80	464.0
128.90	231.0
130.00	467.0
130.70	160.0
131.20	96.0
133.10	200.0
133.70	103.0
135.00	237.0
137.00	153.0
139.80	83.0
141.00	1088.0
142.90	1207.0
143.90	92.0
144.90	174.0
146.10	176.0
146.90	168.0
148.00	171.0
148.80	99.0
150.00	89.0
152.70	80.0
153.00	76.0
154.90	245.0
157.10	176.0
159.00	109.0

Instrument :
MSVOA_W
ClientSampleId :
BFB449

160.90	150.0
162.90	74.0
170.50	61.0
171.00	115.0
171.80	521.0
172.20	511.0
174.00	70712.0
175.10	4840.0
176.00	68952.0
177.00	4057.0
178.00	128.0
179.20	53.0
191.00	273.0
192.90	427.0
194.00	68.0
204.80	59.0
206.90	139.0
207.20	133.0
248.90	177.0
251.10	66.0
264.90	227.0
267.00	138.0
281.10	3234.0
282.00	733.0
283.20	457.0
284.20	90.0

Instrument :
MSVOA_W
ClientSampleId :
BFB449

m/z	Abundance
36.00	728.0
37.00	3634.0
38.10	3310.0
39.00	1595.0
40.00	240.0
44.00	697.0
45.00	579.0
46.10	124.0
47.00	843.0
48.10	410.0
49.00	3432.0
50.00	15160.0
51.10	4484.0
51.90	139.0
55.00	272.0
56.00	1219.0
57.00	2551.0
58.00	69.0
60.10	916.0
61.00	3932.0
62.10	4372.0
63.00	3647.0
64.00	318.0
65.00	270.0
67.00	175.0
68.00	9722.0
69.00	8420.0
70.10	584.0
72.00	520.0
73.00	4315.0
74.10	15380.0
75.00	45152.0
76.10	3786.0
77.00	549.0
77.90	425.0
78.90	3511.0
80.00	1007.0
80.90	3700.0
82.00	838.0
83.00	126.0
86.10	105.0
86.90	3320.0
88.00	2771.0
90.90	448.0
92.00	2723.0
93.00	4161.0
94.00	9228.0
95.00	83136.0
96.10	5578.0
97.10	195.0
103.90	392.0
104.90	212.0
105.90	379.0
106.70	63.0
107.10	58.0
110.00	68.0
110.80	121.0
111.90	155.0
114.90	135.0
115.90	430.0
117.00	601.0
117.90	321.0
118.70	385.0
119.10	448.0
124.00	59.0
125.10	66.0
127.80	328.0
129.10	143.0
129.90	298.0
130.90	199.0
133.00	161.0
134.00	51.0
134.80	245.0
137.00	158.0
139.80	135.0
140.90	1423.0
141.80	166.0
143.00	1027.0
143.80	161.0
144.70	174.0
145.70	118.0
146.10	95.0
146.80	98.0
148.00	186.0
148.90	78.0
149.90	84.0
152.60	85.0
154.00	68.0
155.10	193.0
156.80	152.0
157.90	54.0
159.10	118.0

Instrument :
MSVOA_W
ClientSampleId :
BFB449

160.90	261.0
171.80	333.0
174.00	60192.0
175.00	5920.0
176.00	62552.0
177.00	4180.0
177.90	90.0
193.10	209.0
205.10	89.0
206.90	56.0
207.30	67.0
265.10	106.0
281.10	1391.0
282.00	309.0
283.00	327.0

Instrument :
MSVOA_W
ClientSampleId :
BFB449