

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110424\
 Data File : VW030907.D
 Acq On : 04 Nov 2024 15:31
 Operator : SY/MD
 Sample : VW1104SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 05 00:40:37 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Nov 05 00:39:41 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	449129	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	418340	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	191677	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	153401	20.825	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.320%
7) Chloroethane-d5	2.899	69	126140	22.328	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.320%
11) 1,1-Dichloroethene-d2	4.021	65	67882	22.333	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	89.320%
21) 2-Butanone-d5	7.075	46	68620	56.608	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	113.220%
24) Chloroform-d	7.648	84	322877	24.386	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.560%
26) 1,2-Dichloroethane-d4	8.301	65	170843	25.952	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	103.800%
32) Benzene-d6	8.270	84	638316	24.561	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	98.240%
36) 1,2-Dichloropropane-d6	9.270	67	187373	24.457	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.840%
41) Toluene-d8	10.319	98	569017	24.409	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	97.640%
43) trans-1,3-Dichloroprop...	10.575	79	75905	24.442	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	97.760%
47) 2-Hexanone-d5	10.922	63	55403	55.798	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	111.600%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	142461	26.689	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	106.760%
66) 1,2-Dichlorobenzene-d4	13.848	152	177727	25.455	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	101.800%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	5461	0.542	ug/L	# 59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110424\
Data File : VW030907.D
Acq On : 04 Nov 2024 15:31
Operator : SY/MD
Sample : VW1104SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Nov 05 00:40:37 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Nov 05 00:39:41 2024
Response via : Initial Calibration

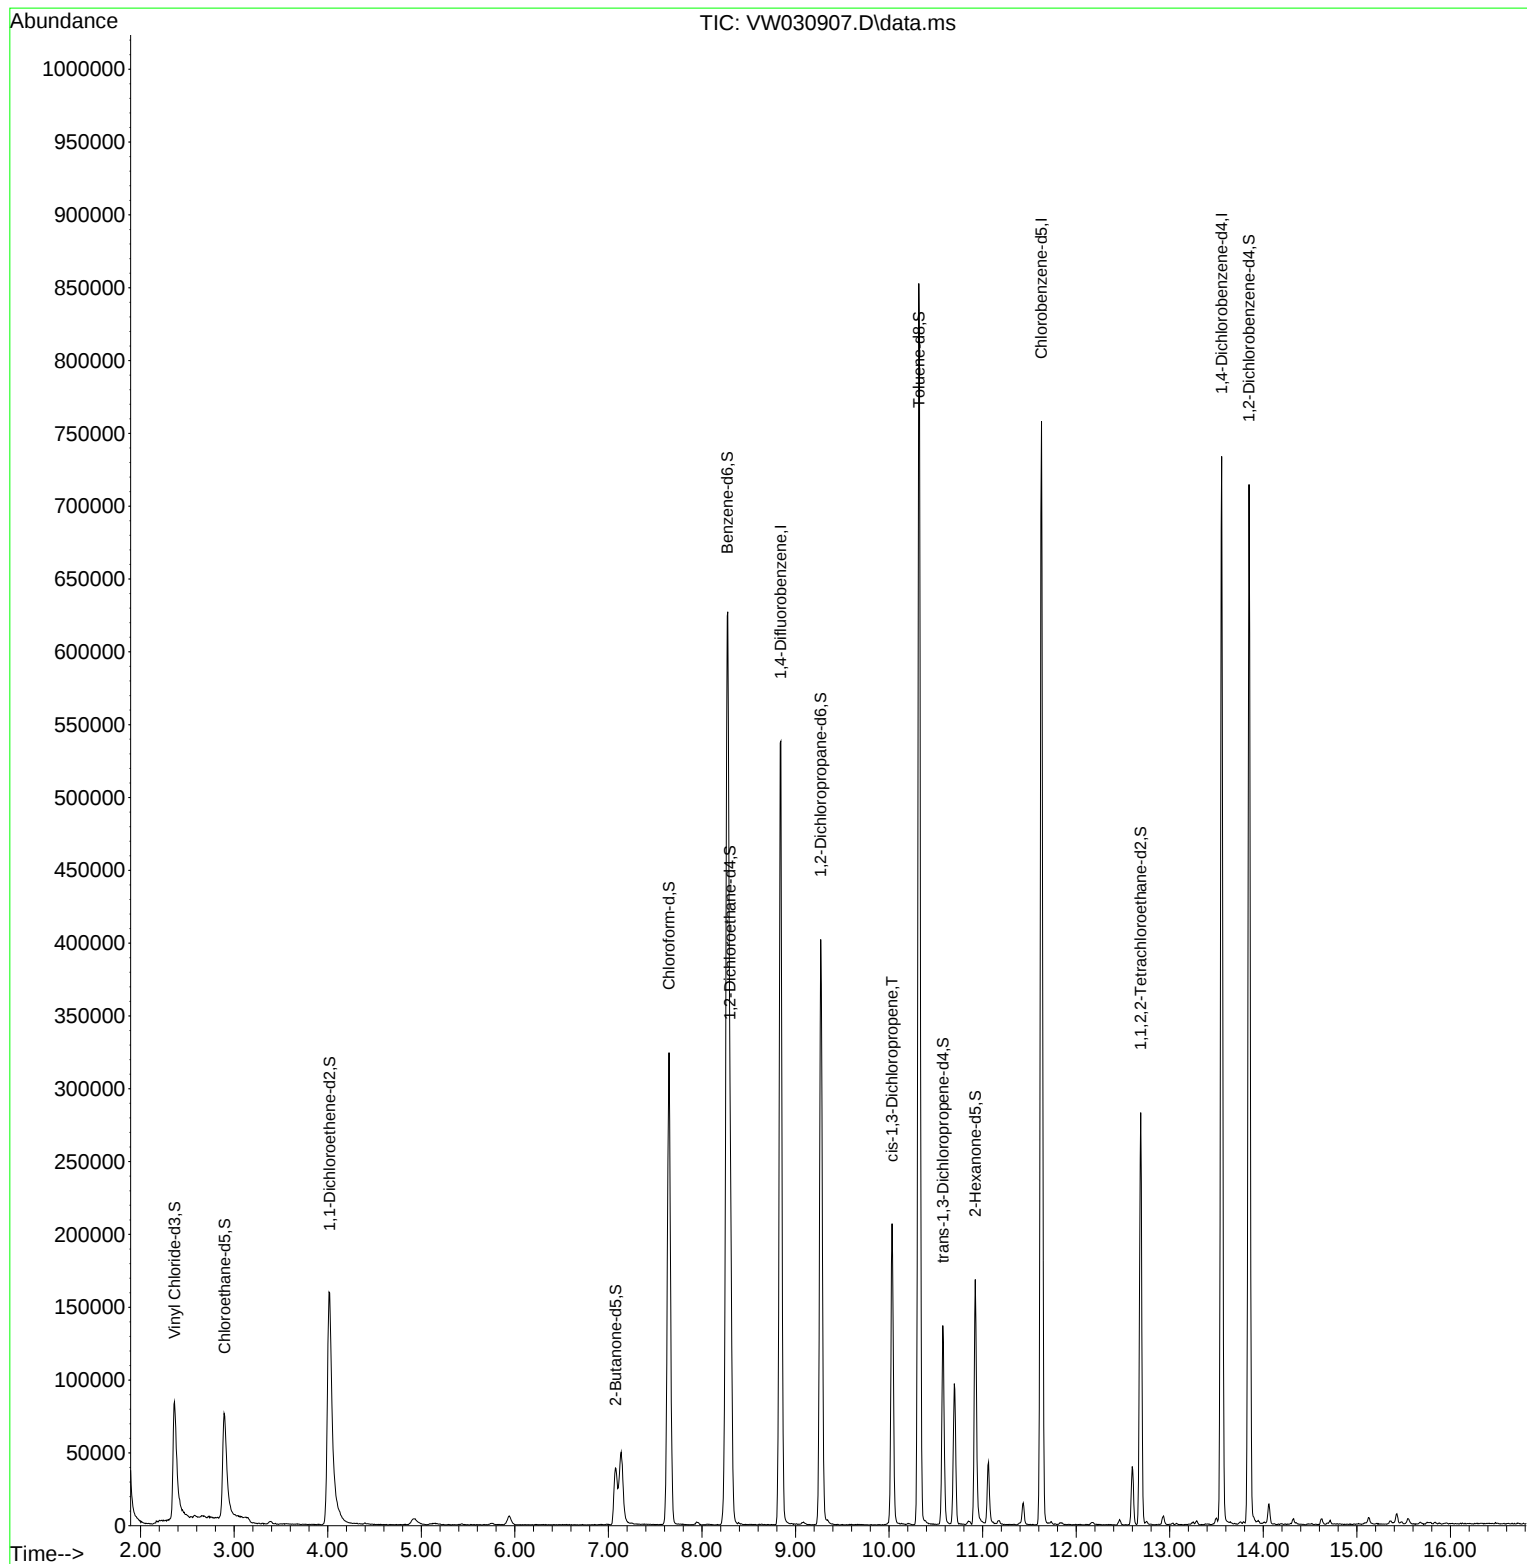

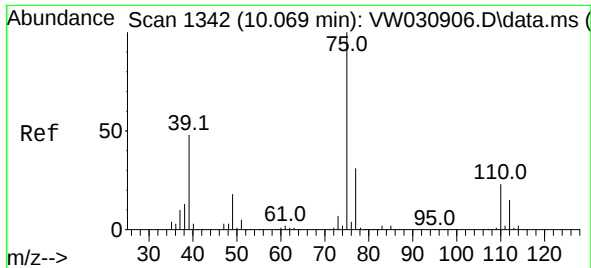

#39
cis-1,3-Dichloropropene
Concen: 0.542 ug/L
RT: 10.032 min Scan# 14
Delta R.T. -0.037 min
Lab File: VW030907.D
Acq: 04 Nov 2024 15:31

Instrument :
MSVOA_W
ClientSampleId :

Tgt Ion: 75 Resp: 5461
Ion Ratio Lower Upper
75 100
77 53.0 21.3 39.6#

