

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110424\
 Data File : VW030908.D
 Acq On : 04 Nov 2024 16:12
 Operator : SY/MD
 Sample : P4622-01
 Misc : 3.99g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 05 00:40:53 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Nov 05 00:39:41 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	445502	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	408655	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	181997	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	182900	25.032	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	100.120%
7) Chloroethane-d5	2.893	69	131152	23.404	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.600%
11) 1,1-Dichloroethene-d2	4.015	65	72340	23.994	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	95.960%
21) 2-Butanone-d5	7.075	46	73540	61.160	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	122.320%
24) Chloroform-d	7.648	84	299350	22.793	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.160%
26) 1,2-Dichloroethane-d4	8.301	65	163138	24.983	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	99.920%
32) Benzene-d6	8.270	84	577518	22.748	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	91.000%
36) 1,2-Dichloropropane-d6	9.270	67	170787	22.820	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.280%
41) Toluene-d8	10.319	98	522568	22.948	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	91.800%
43) trans-1,3-Dichloroprop...	10.575	79	72006	23.736	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	94.960%
47) 2-Hexanone-d5	10.922	63	56502	58.253	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	116.500%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	143965	27.610	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	110.440%
66) 1,2-Dichlorobenzene-d4	13.849	152	170172	25.669	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.680%
Target Compounds						
39) cis-1,3-Dichloropropene	10.032	75	5236	0.532	ug/L	Qvalue # 62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110424\
Data File : VW030908.D
Acq On : 04 Nov 2024 16:12
Operator : SY/MD
Sample : P4622-01
Misc : 3.99g/10mL/MSVOA_W/SOIL/A
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Nov 05 00:40:53 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Nov 05 00:39:41 2024
Response via : Initial Calibration

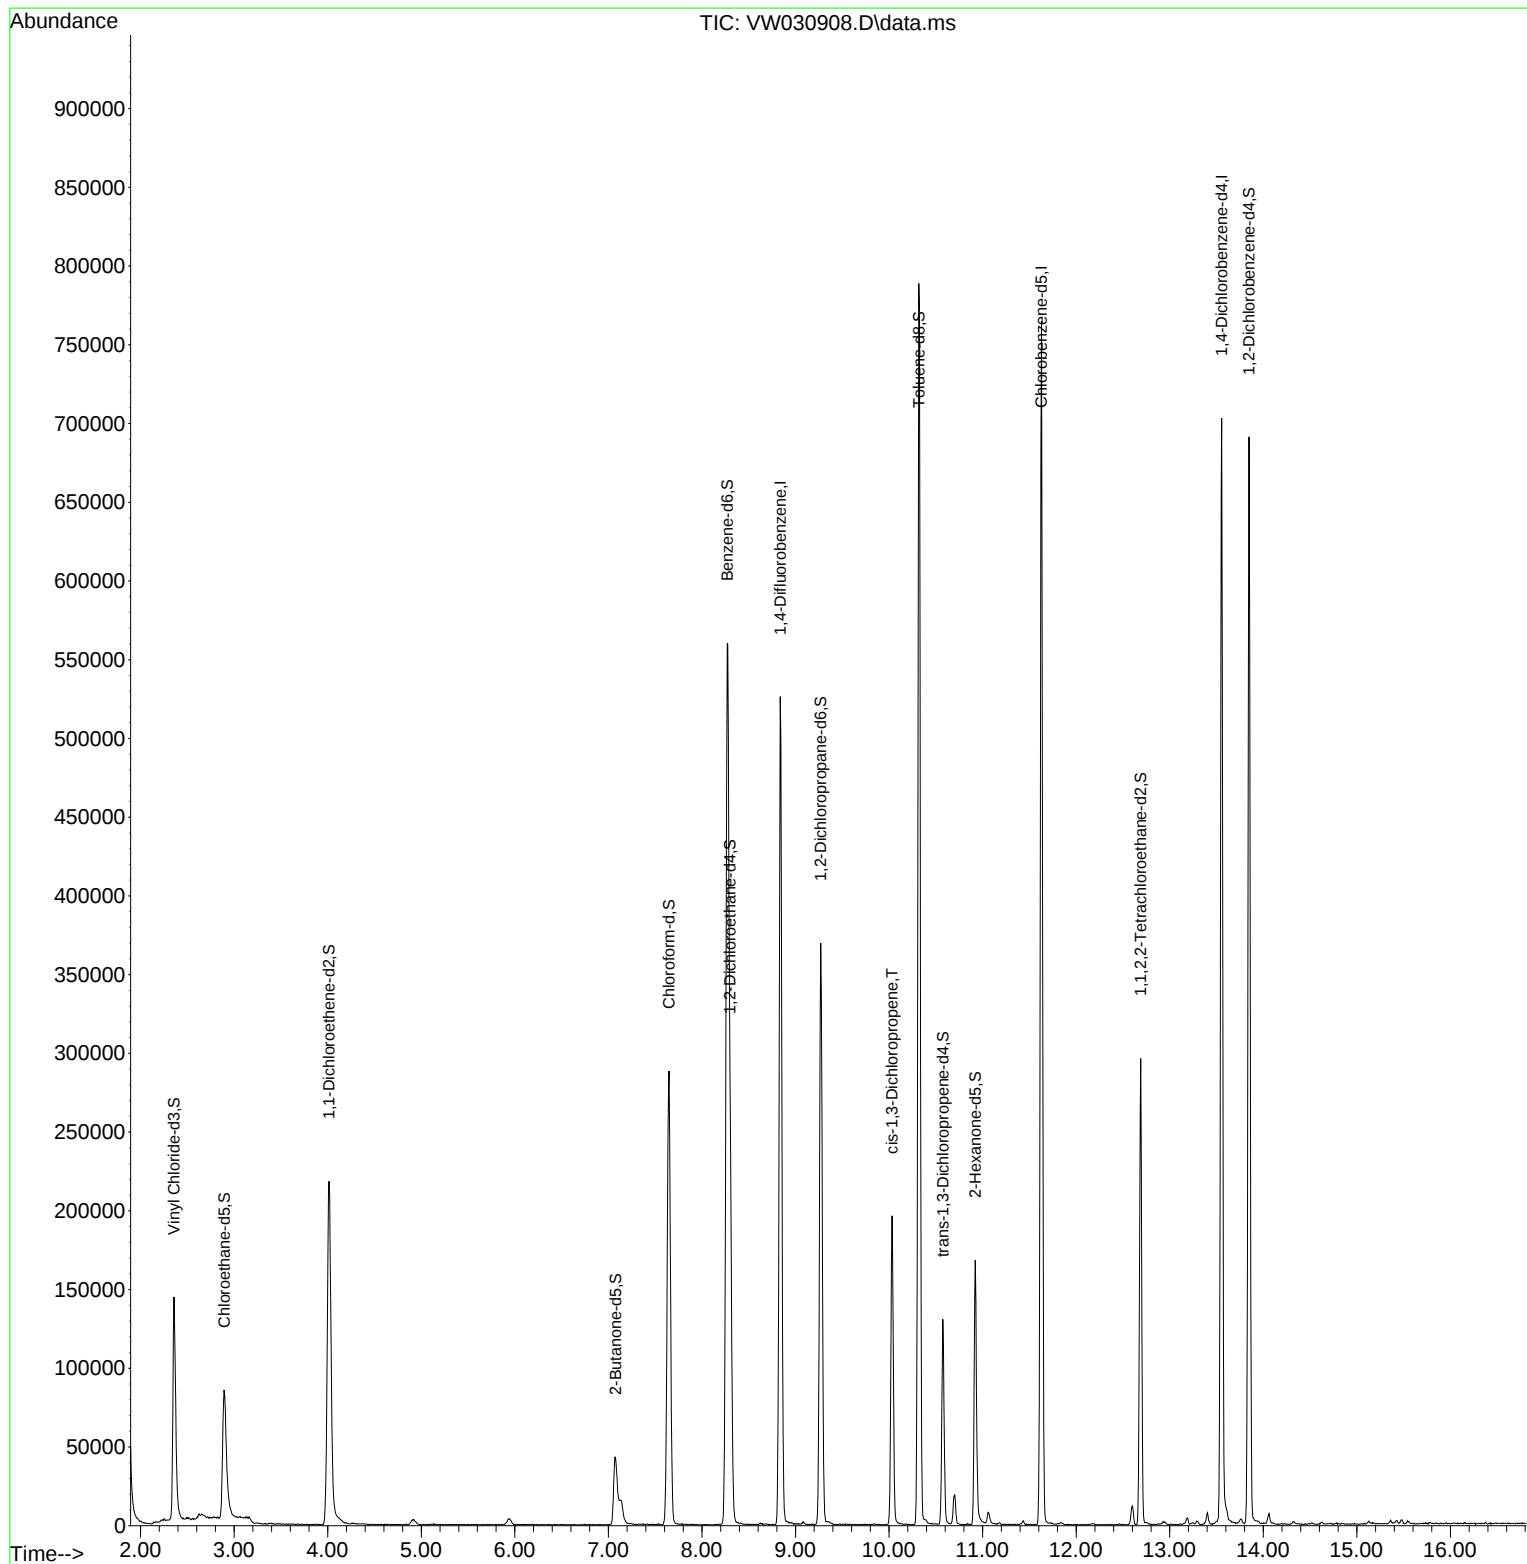

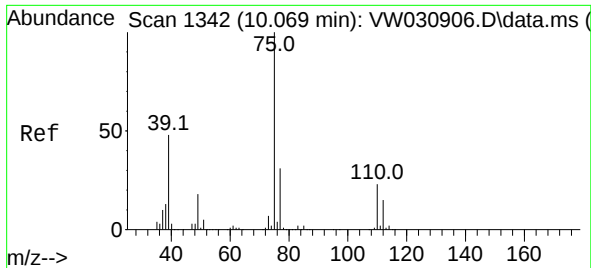

#39
cis-1,3-Dichloropropene
Concen: 0.532 ug/L
RT: 10.032 min Scan# 14
Delta R.T. -0.036 min
Lab File: VW030908.D
Acq: 04 Nov 2024 16:12

Instrument :
MSVOA_W
ClientSampleId :

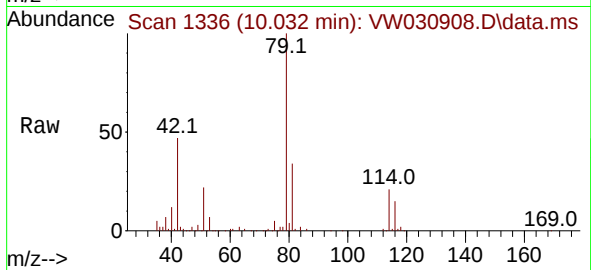

Tgt Ion: 75 Resp: 5236
Ion Ratio Lower Upper
75 100
77 51.5 21.3 39.6#

