

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110424\
 Data File : VW030911.D
 Acq On : 04 Nov 2024 17:24
 Operator : SY/MD
 Sample : P4622-04
 Misc : 3.26g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 05 00:41:35 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Nov 05 00:39:41 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	629186	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	553908	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	238526	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	243414	23.588	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	94.360%
7) Chloroethane-d5	2.899	69	182510	23.061	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	92.240%
11) 1,1-Dichloroethene-d2	4.021	65	102777	24.137	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	96.560%
21) 2-Butanone-d5	7.075	46	110813	65.254	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	130.500%
24) Chloroform-d	7.648	84	426377	22.987	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.960%
26) 1,2-Dichloroethane-d4	8.307	65	237142	25.714	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	102.840%
32) Benzene-d6	8.276	84	852321	24.769	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	99.080%
36) 1,2-Dichloropropane-d6	9.270	67	250979	24.741	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	98.960%
41) Toluene-d8	10.325	98	746604	24.189	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	96.760%
43) trans-1,3-Dichloroprop...	10.575	79	104790	25.485	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	101.920%
47) 2-Hexanone-d5	10.922	63	87258	66.371	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	132.740%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	207150	29.310	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	117.240%
66) 1,2-Dichlorobenzene-d4	13.848	152	229794	26.448	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	105.800%
Target Compounds						Qvalue
34) Trichloroethene	8.843	95	18958	1.926	ug/L	# 4


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110424\
Data File : VW030911.D
Acq On : 04 Nov 2024 17:24
Operator : SY/MD
Sample : P4622-04
Misc : 3.26g/10mL/MSVOA_W/SOIL/A
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Nov 05 00:41:35 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Nov 05 00:39:41 2024
Response via : Initial Calibration

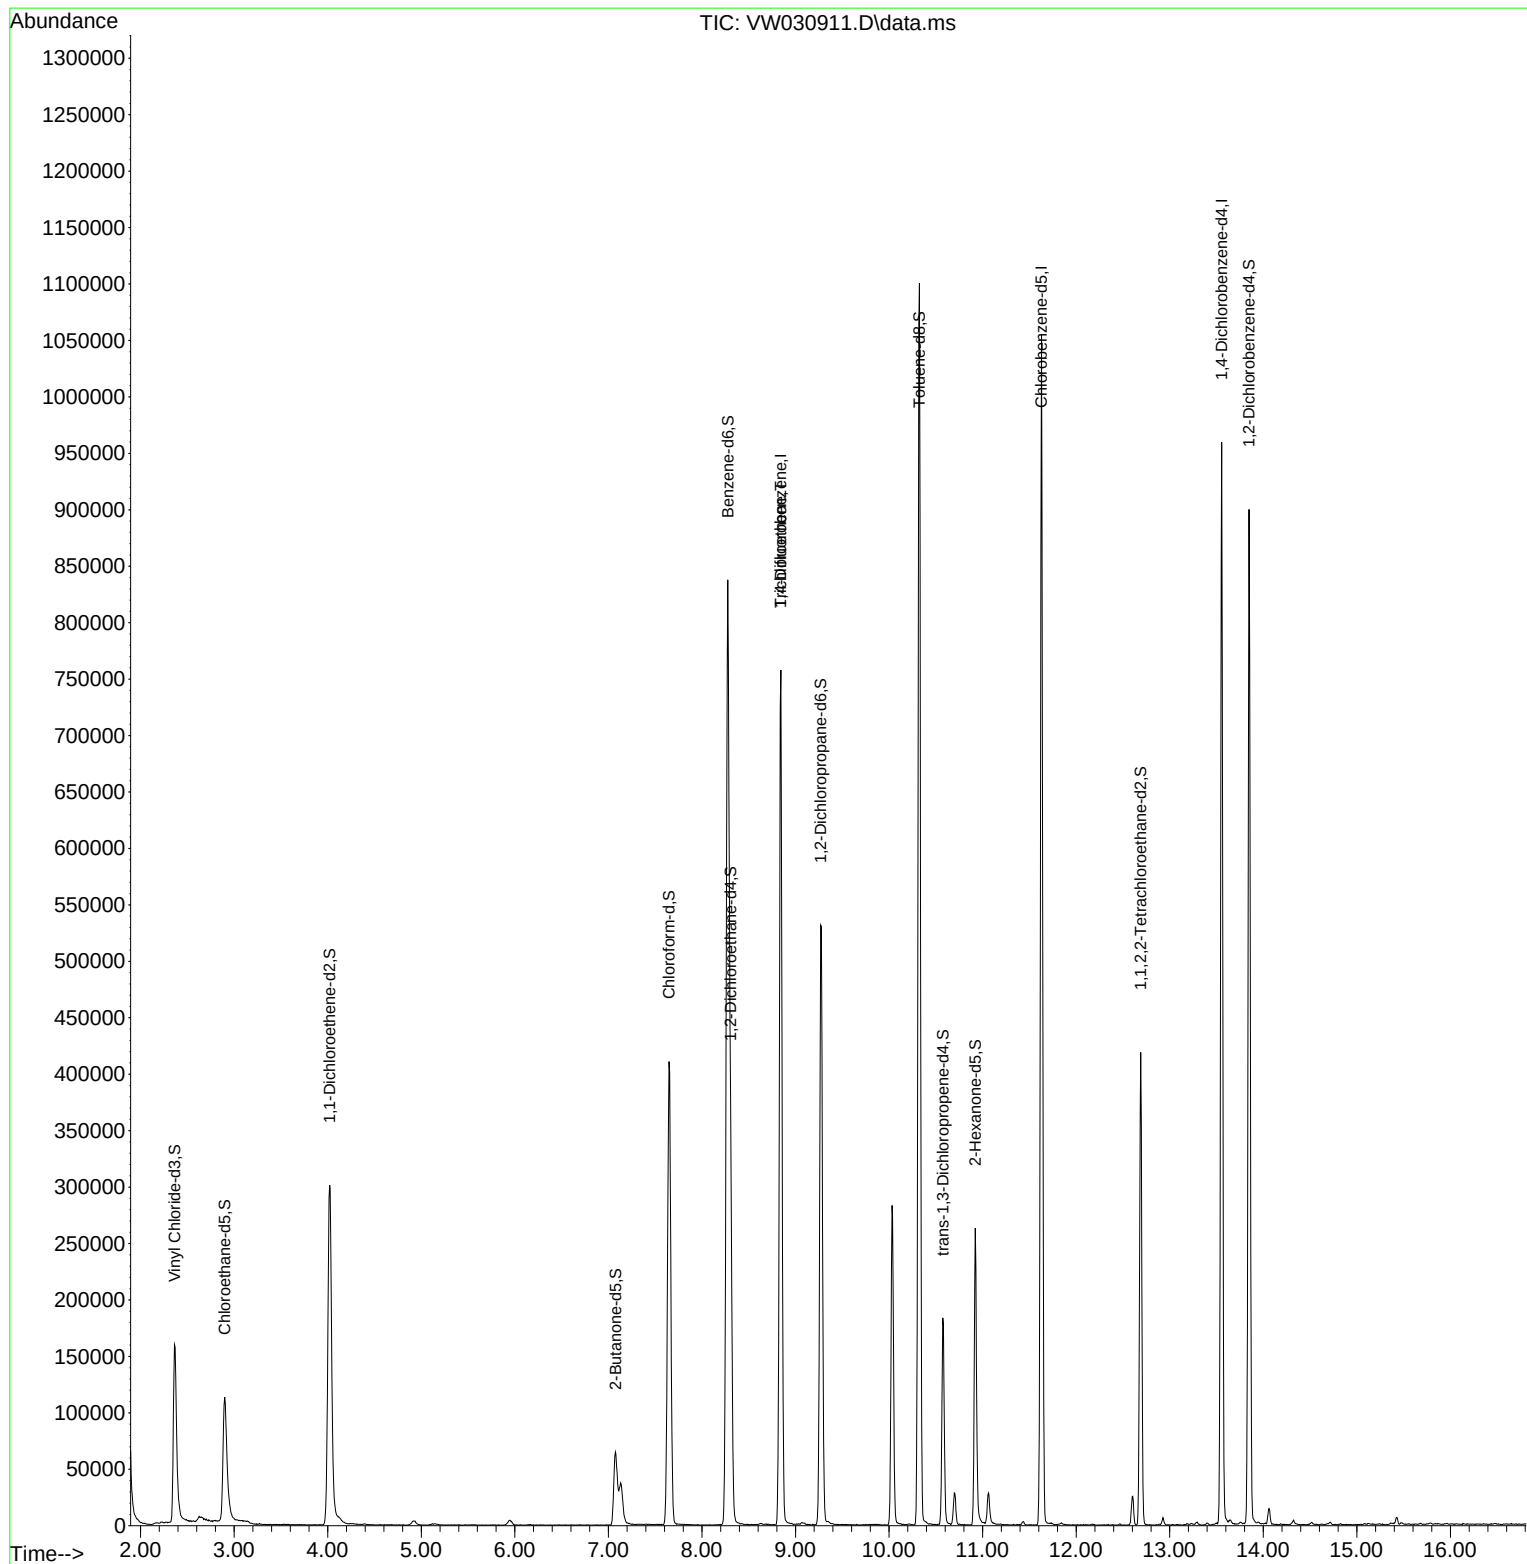

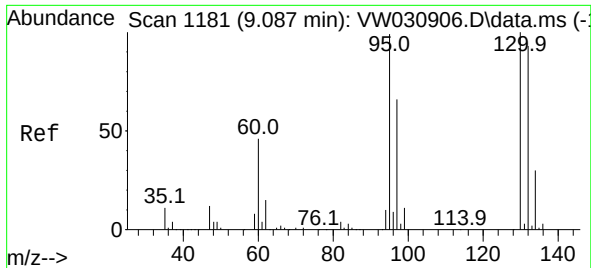

#34
 Trichloroethene
 Concen: 1.926 ug/L
 RT: 8.843 min Scan# 11
 Delta R.T. -0.244 min
 Lab File: VW030911.D
 Acq: 04 Nov 2024 17:24

Instrument :
 MSVOA_W
 ClientSampleId :

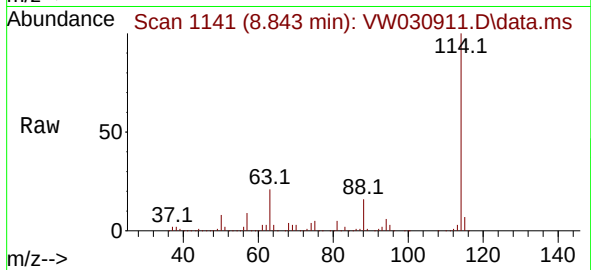

Tgt Ion: 95 Resp: 18958

Ion	Ratio	Lower	Upper
95	100		
97	0.0	48.9	90.7#
132	0.0	67.7	125.7#
130	0.0	73.1	135.8#

