

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110424\
 Data File : VW030916.D
 Acq On : 04 Nov 2024 19:25
 Operator : SY/MD
 Sample : P4622-09
 Misc : 4.15g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 05 00:42:49 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Nov 05 00:39:41 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	631829	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	585301	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	267246	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	228340	22.035	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	88.160%		
7) Chloroethane-d5	2.893	69	165408	20.812	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	83.240%		
11) 1,1-Dichloroethene-d2	4.021	65	90654	21.201	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	84.800%		
21) 2-Butanone-d5	7.075	46	96464	56.567	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	113.140%		
24) Chloroform-d	7.648	84	397875	21.361	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	85.440%		
26) 1,2-Dichloroethane-d4	8.301	65	214281	23.138	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	92.560%		
32) Benzene-d6	8.270	84	790733	21.746	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	87.000%		
36) 1,2-Dichloropropane-d6	9.270	67	237412	22.148	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	88.600%		
41) Toluene-d8	10.325	98	719809	22.070	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	88.280%		
43) trans-1,3-Dichloroprop...	10.575	79	95951	22.083	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	88.320%		
47) 2-Hexanone-d5	10.922	63	76676	55.194	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	110.380%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	188692	25.266	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	101.080%		
66) 1,2-Dichlorobenzene-d4	13.849	152	231624	23.794	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	95.160%		
Target Compounds						Qvalue
34) Trichloroethene	8.843	95	19379	1.863	ug/L	# 4


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110424\
Data File : VW030916.D
Acq On : 04 Nov 2024 19:25
Operator : SY/MD
Sample : P4622-09
Misc : 4.15g/10mL/MSVOA_W/SOIL/A
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Nov 05 00:42:49 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Nov 05 00:39:41 2024
Response via : Initial Calibration

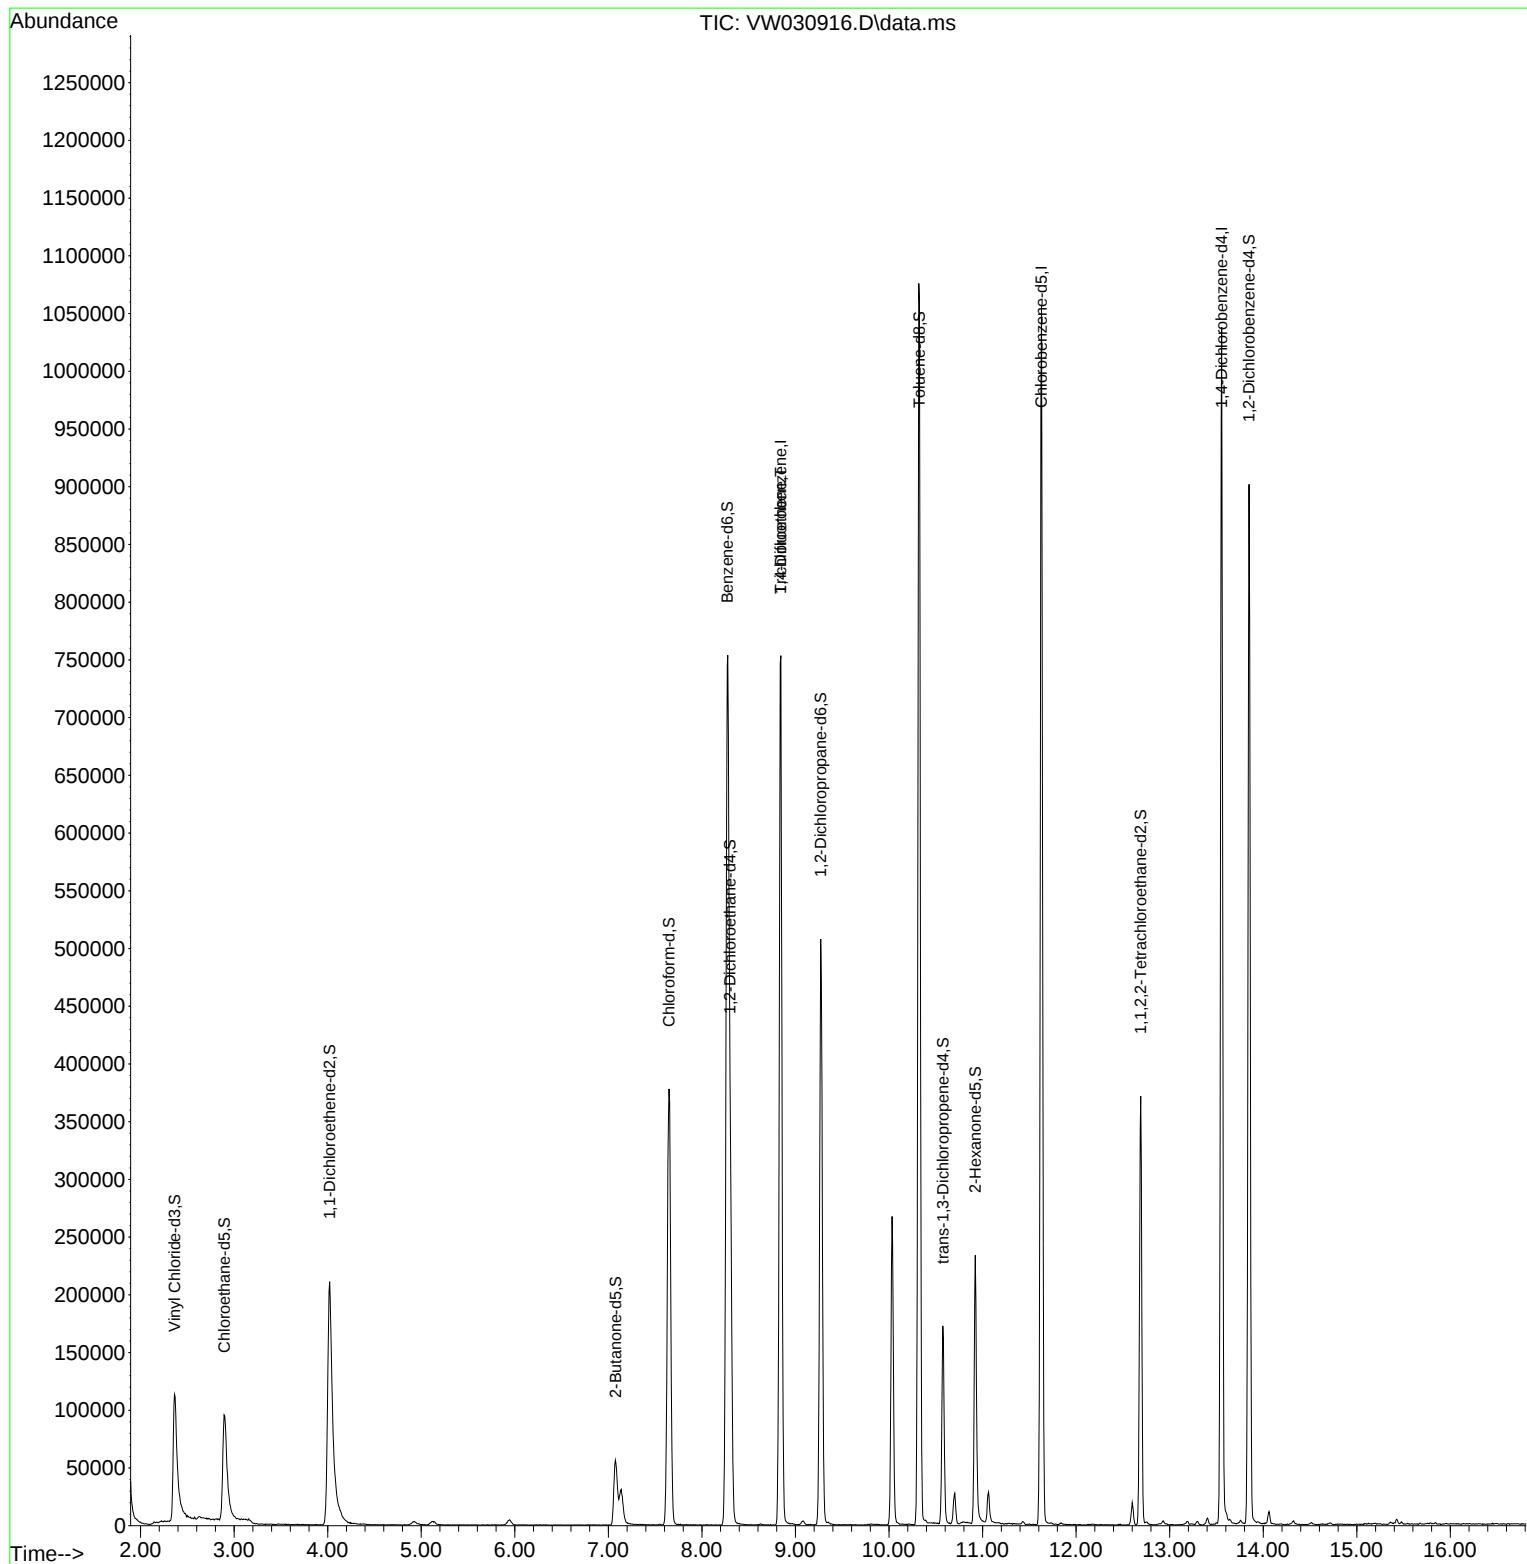

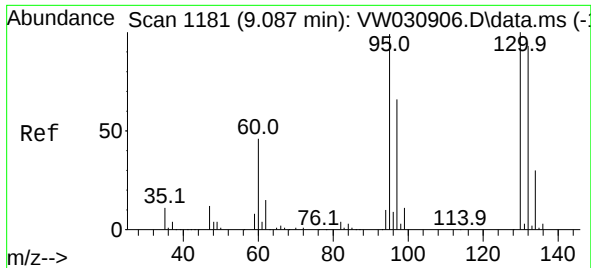

#34
 Trichloroethene
 Concen: 1.863 ug/L
 RT: 8.843 min Scan# 11
 Delta R.T. -0.244 min
 Lab File: VW030916.D
 Acq: 04 Nov 2024 19:25

Instrument :
 MSVOA_W
 ClientSampleId :

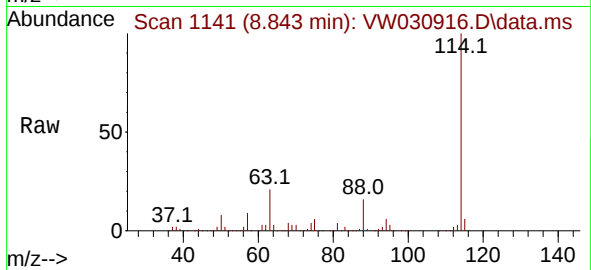

Tgt Ion: 95 Resp: 19379

Ion	Ratio	Lower	Upper
95	100		
97	0.0	48.9	90.7#
132	0.0	67.7	125.7#
130	0.0	73.1	135.8#

