

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110424\
 Data File : VW030917.D
 Acq On : 04 Nov 2024 19:49
 Operator : SY/MD
 Sample : P4622-10
 Misc : 5.27g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 05 00:43:04 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Nov 05 00:39:41 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	631396	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	550751	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	220077	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	224511	21.680	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	86.720%
7) Chloroethane-d5	2.893	69	169340	21.322	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.280%
11) 1,1-Dichloroethene-d2	4.015	65	92653	21.684	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	86.720%
21) 2-Butanone-d5	7.075	46	106322	62.390	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	124.780%
24) Chloroform-d	7.648	84	414736	22.281	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.120%
26) 1,2-Dichloroethane-d4	8.307	65	230056	24.858	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	99.440%
32) Benzene-d6	8.276	84	825834	24.136	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	96.560%
36) 1,2-Dichloropropane-d6	9.270	67	244687	24.259	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.040%
41) Toluene-d8	10.318	98	704285	22.948	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	91.800%
43) trans-1,3-Dichloroprop...	10.575	79	101935	24.932	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	99.720%
47) 2-Hexanone-d5	10.922	63	80551	61.621	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	123.240%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	198592	28.260	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	113.040%
66) 1,2-Dichlorobenzene-d4	13.854	152	200520	25.013	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.040%
Target Compounds						
39) cis-1,3-Dichloropropene	10.032	75	6882	0.519	ug/L	Qvalue # 57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110424\
Data File : VW030917.D
Acq On : 04 Nov 2024 19:49
Operator : SY/MD
Sample : P4622-10
Misc : 5.27g/10mL/MSVOA_W/SOIL/A
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Nov 05 00:43:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Nov 05 00:39:41 2024
Response via : Initial Calibration

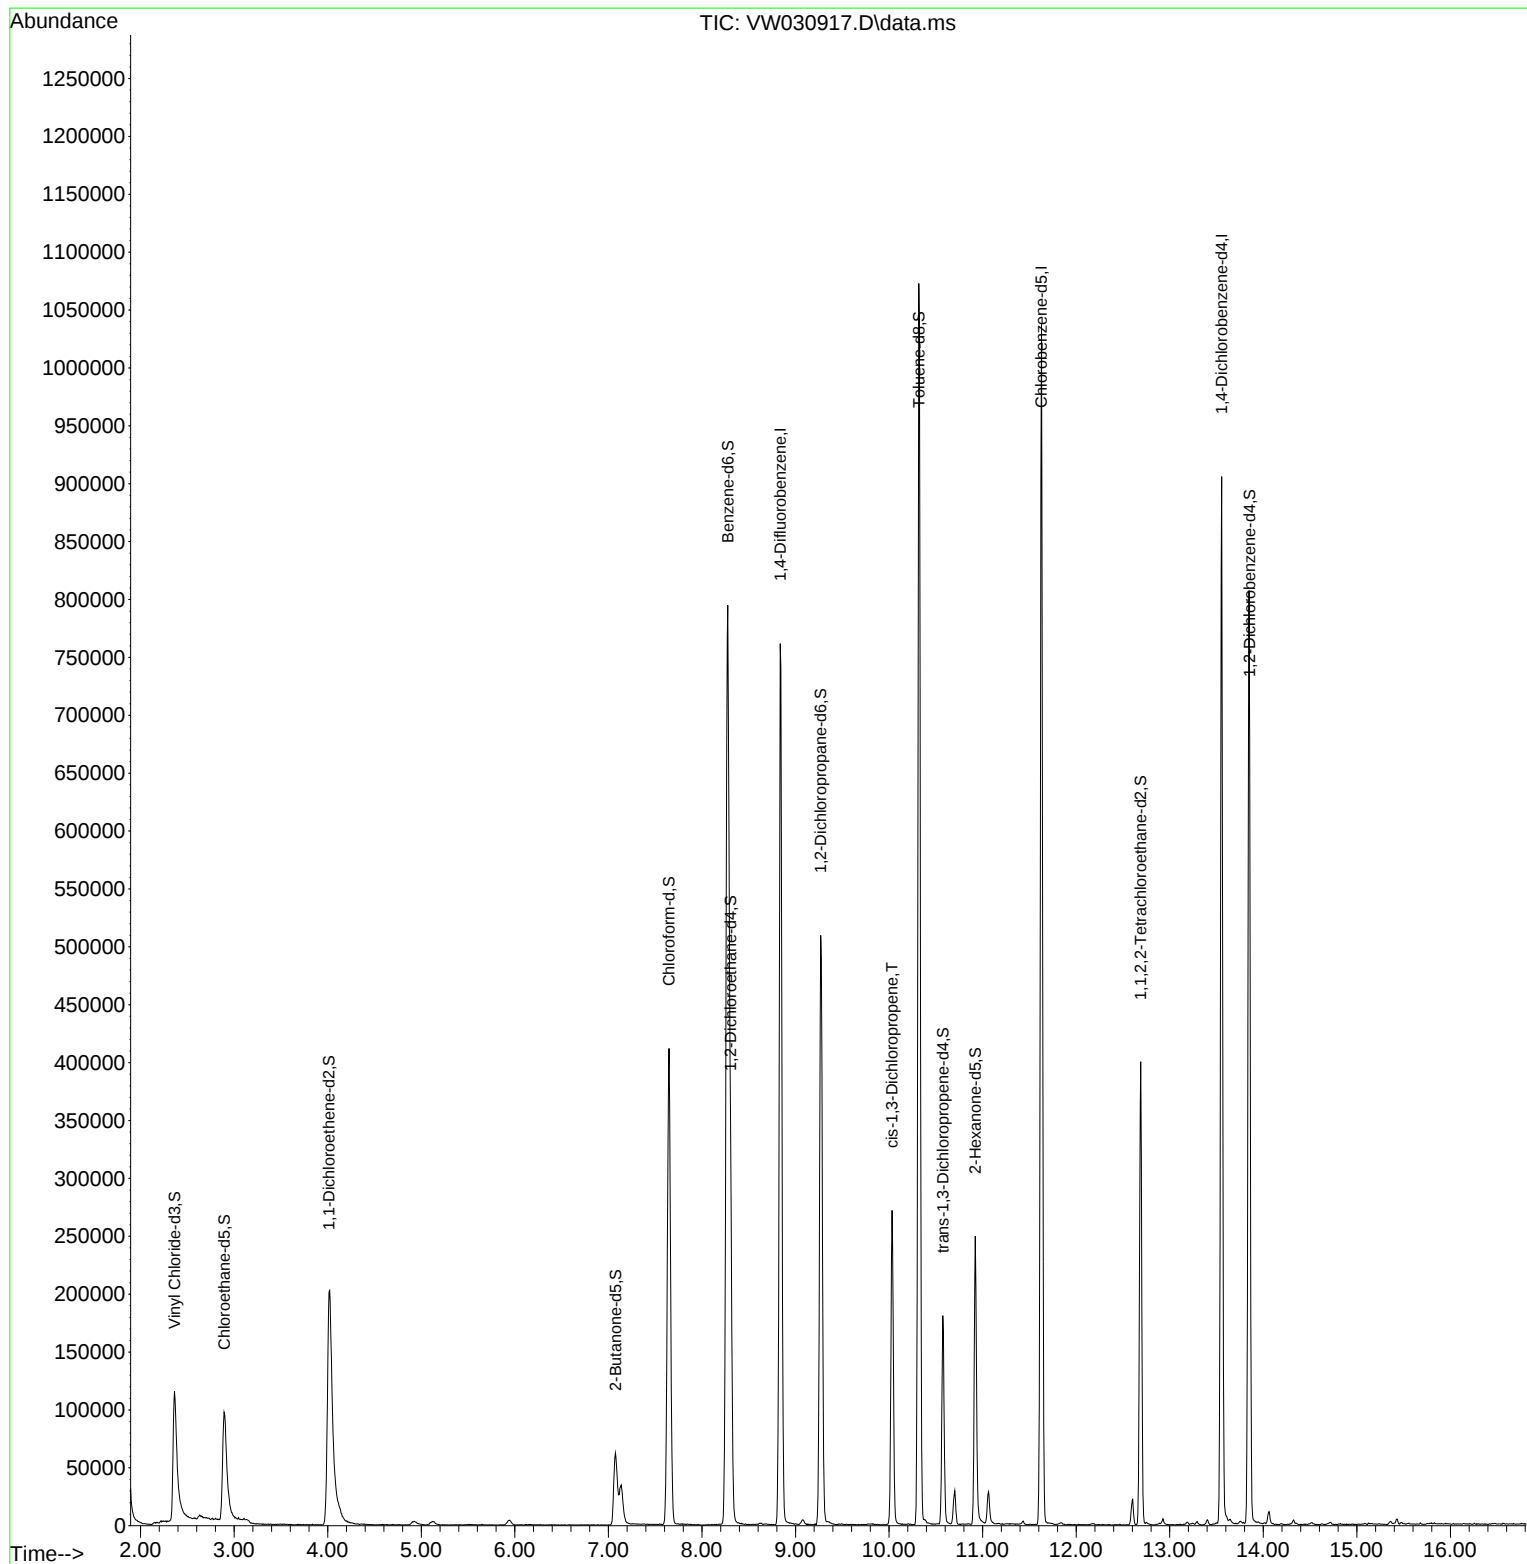

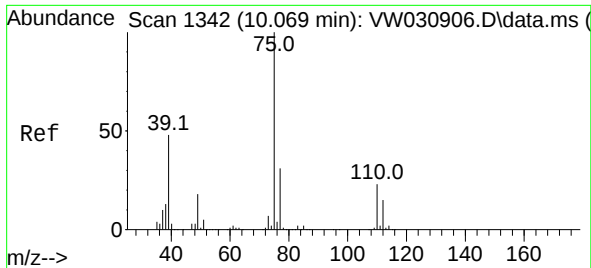

#39
 cis-1,3-Dichloropropene
 Concen: 0.519 ug/L
 RT: 10.032 min Scan# 14
 Delta R.T. -0.037 min
 Lab File: VW030917.D
 Acq: 04 Nov 2024 19:49

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 6882
 Ion Ratio Lower Upper
 75 100
 77 54.0 21.3 39.6#

