

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110621\
 Data File : VW020789.D
 Acq On : 05 Nov 2021 19:12
 Operator : SY/VA
 Sample : M4464-03MSD
 Misc : 6.82g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GB7K1MSD

Manual IntegrationsAPPROVED

Quant Time: Nov 08 04:54:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110621SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Nov 08 04:38:07 2021
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 11/08/2021
 Supervised By :Mahesh Dadoda 11/10/2021

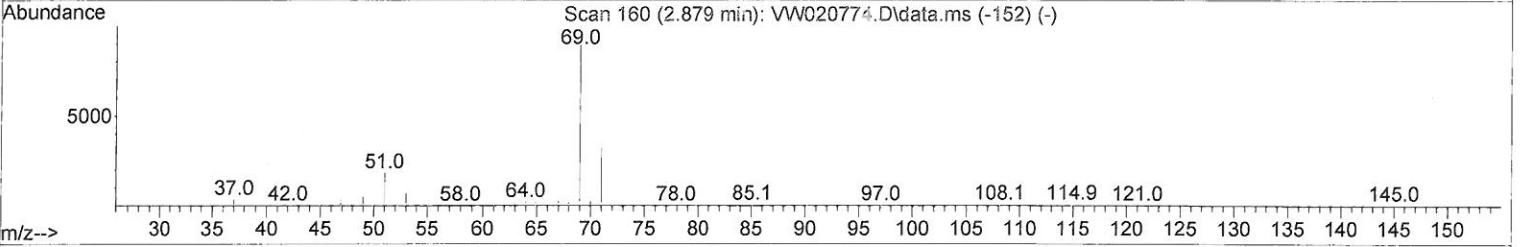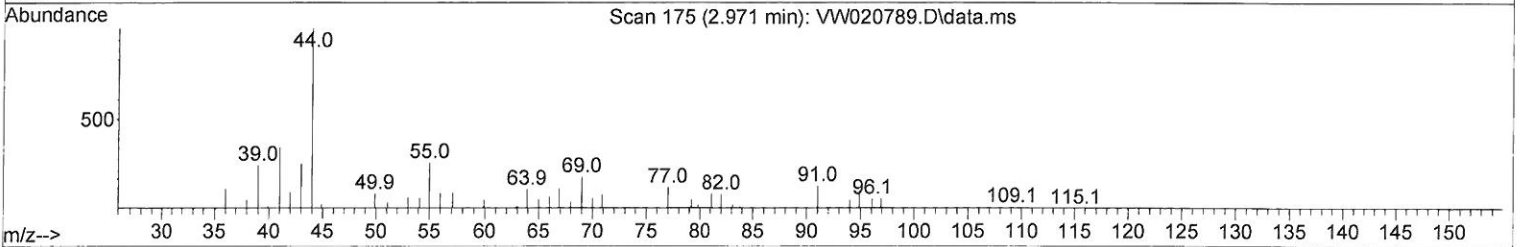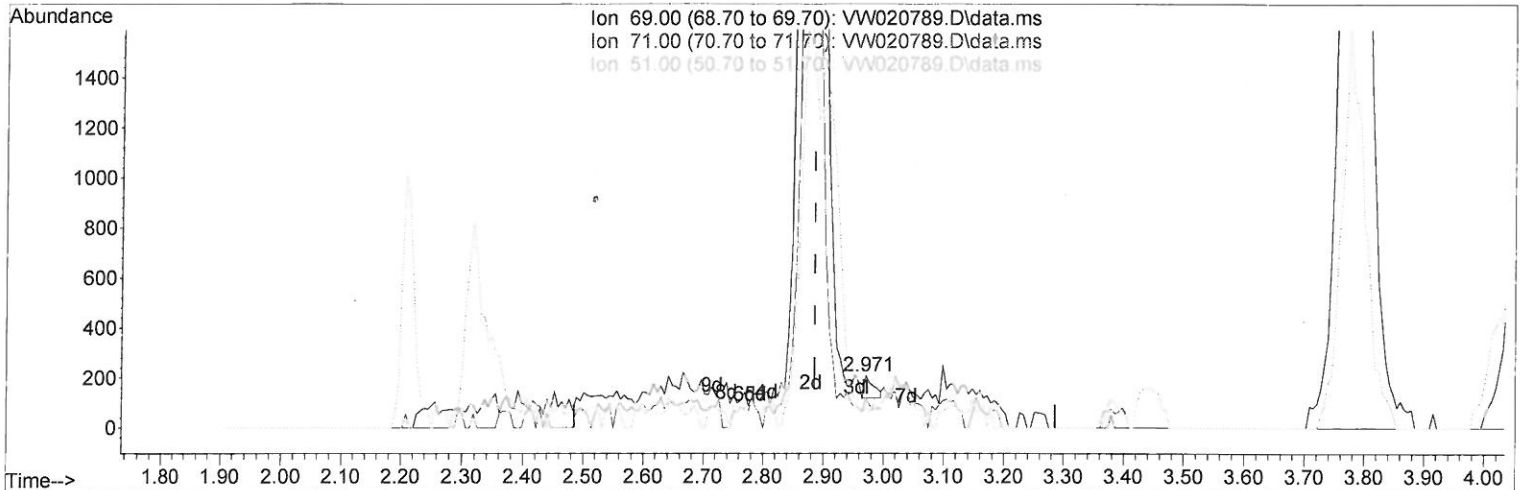

TIC: VW020789.D\data.ms

(7) Chloroethane-d5 (S)

2.971min (+ 0.086) 0.14 ug/L

response 97

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.40	34.02
51.00	29.70	30.93
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110621\
 Data File : VW020789.D
 Acq On : 05 Nov 2021 19:12
 Operator : SY/VA
 Sample : M4464-03MSD
 Misc : 6.82g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GB7K1MSD

Manual IntegrationsAPPROVED

Quant Time: Nov 08 04:54:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110621SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Nov 08 04:38:07 2021
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 11/08/2021
 Supervised By :Mahesh Dadoda 11/10/2021

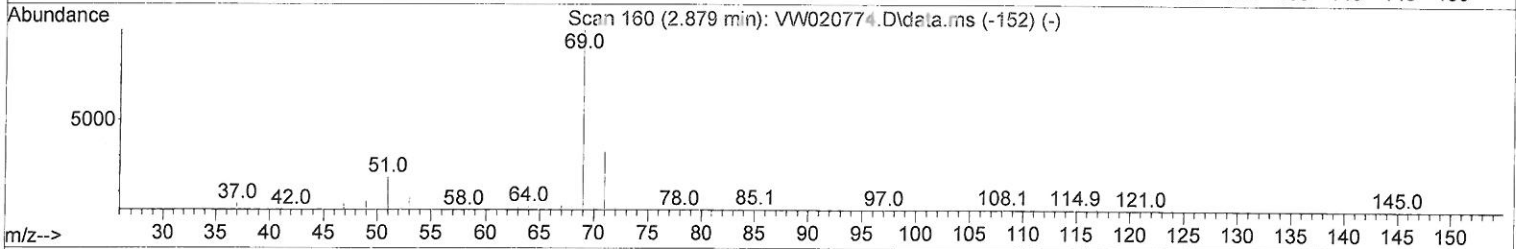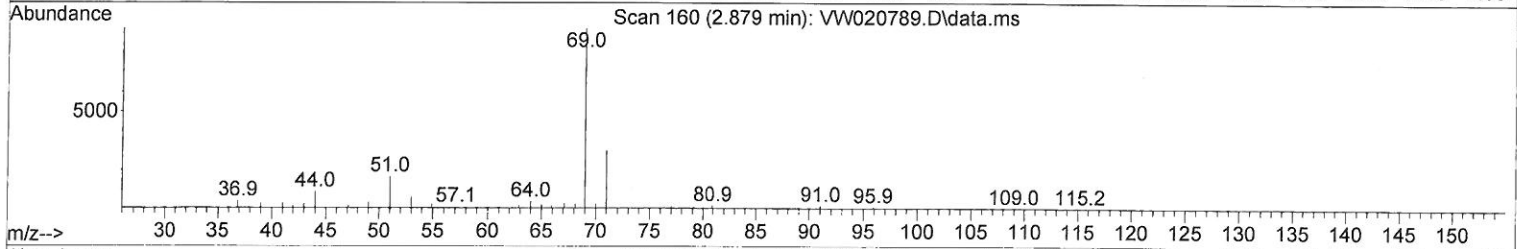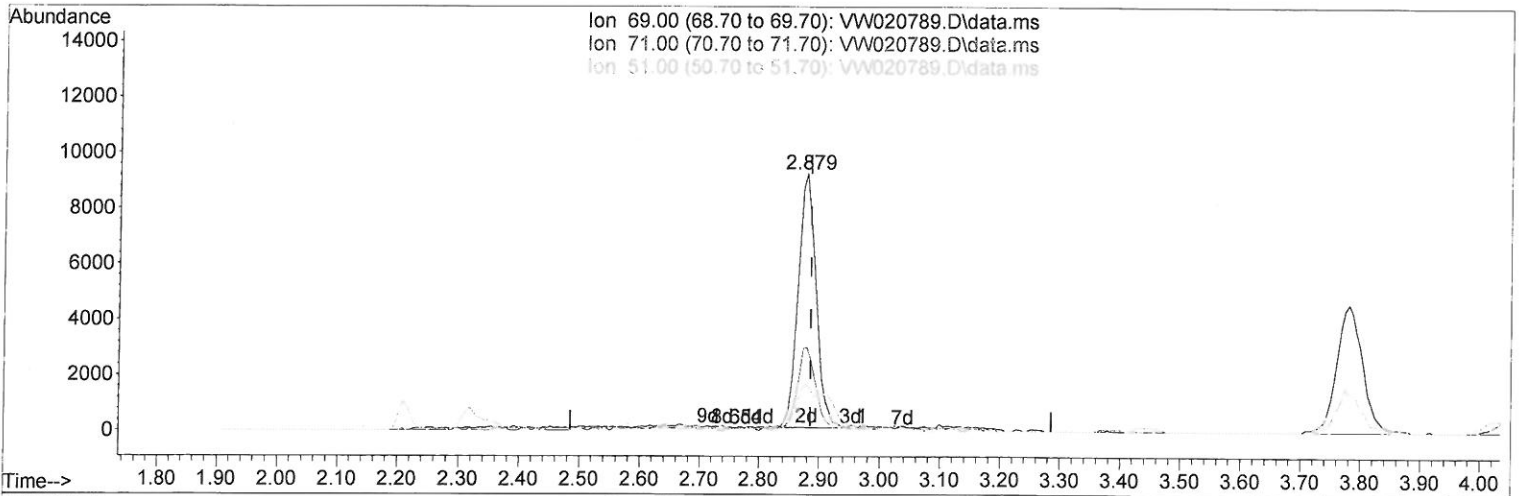

TIC: VW020789.D\data.ms

(7) Chloroethane-d5 (S)

2.879min (-0.006) 27.57 ug/L m

response 18866

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.40	0.17#
51.00	29.70	0.16#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110621\
 Data File : VW020789.D
 Acq On : 05 Nov 2021 19:12
 Operator : SY/VA
 Sample : M4464-03MSD
 Misc : 6.82g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GB7K1MSD

Manual IntegrationsAPPROVED

Quant Time: Nov 08 04:54:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110621SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Nov 08 04:38:07 2021
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 11/08/2021
 Supervised By :Mahesh Dadoda 11/10/2021

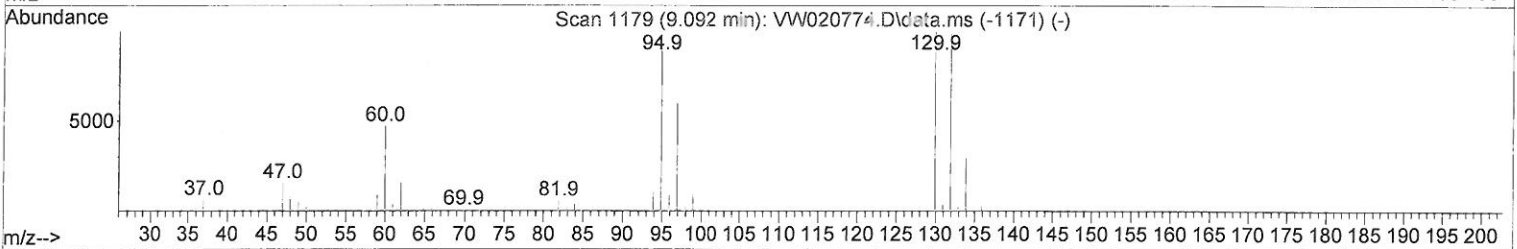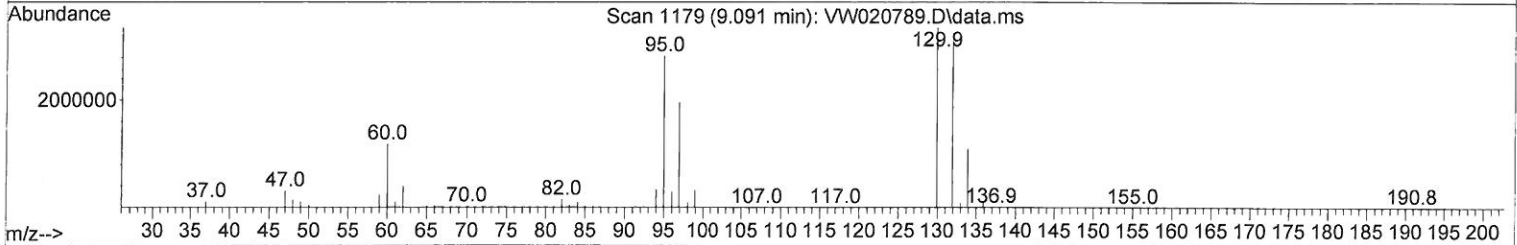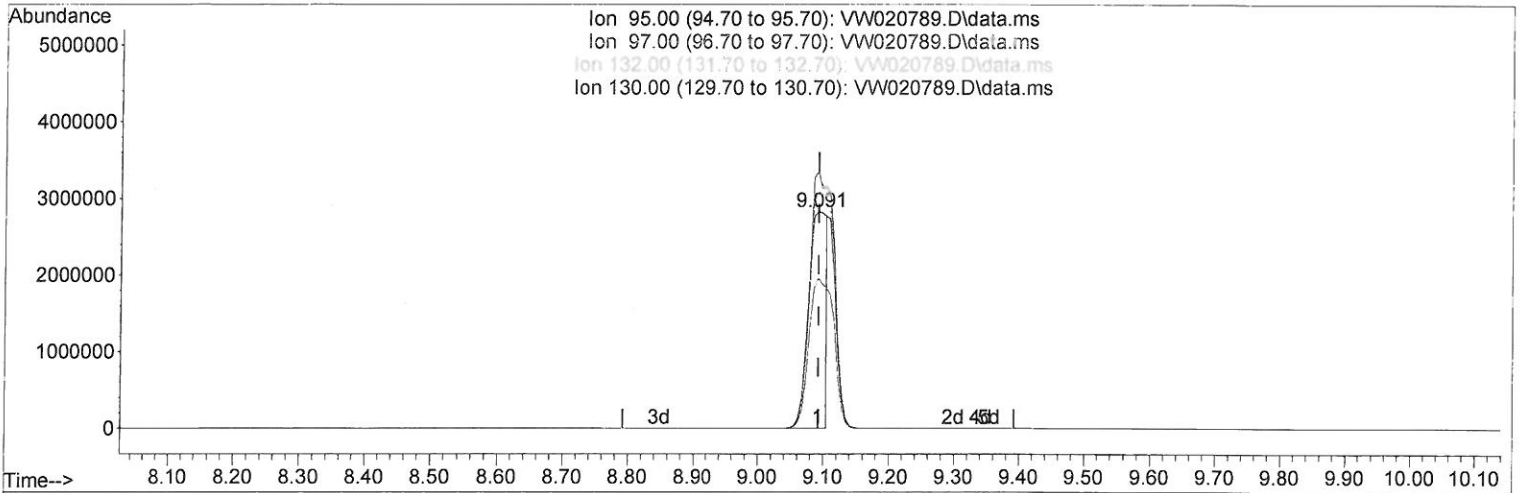

TIC: VW020789.D\data.ms

(34) Trichloroethene (T)

9.091min (-0.000) 3321.93 ug/L

response 5439177

Ion	Exp%	Act%
95.00	100.00	100.00
97.00	67.10	69.19
132.00	93.50	109.85
130.00	99.10	118.52

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110621\
 Data File : VW020789.D
 Acq On : 05 Nov 2021 19:12
 Operator : SY/VA
 Sample : M4464-03MSD
 Misc : 6.82g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GB7K1MSD

Manual IntegrationsAPPROVED

Quant Time: Nov 08 04:54:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110621SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Nov 08 04:38:07 2021
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 11/08/2021
 Supervised By :Mahesh Dadoda 11/10/2021

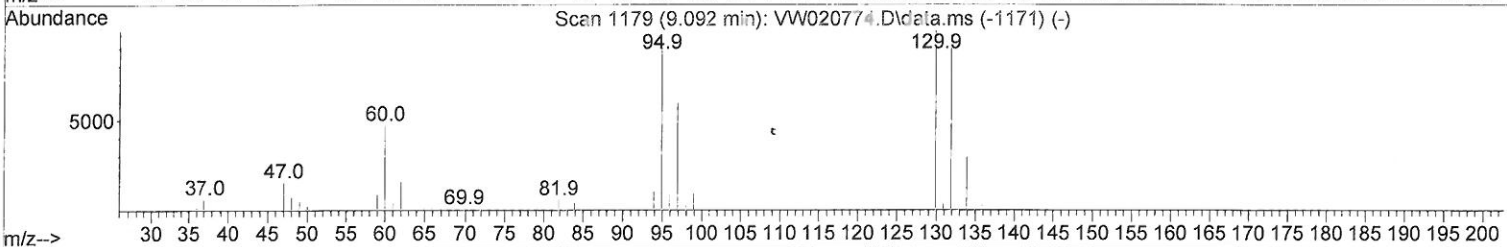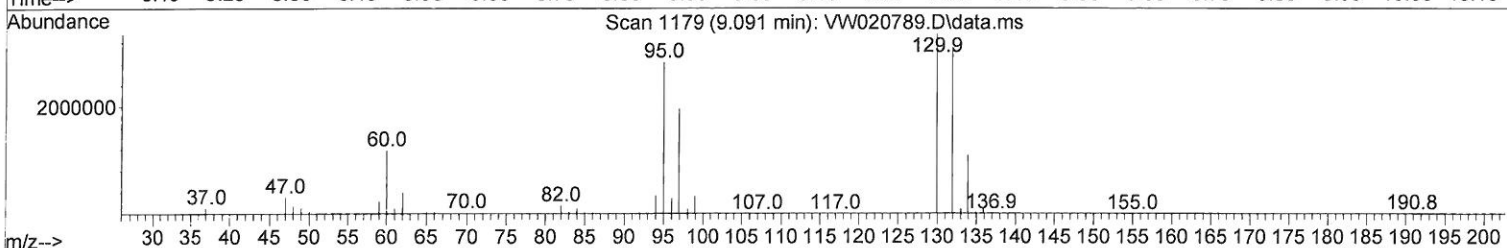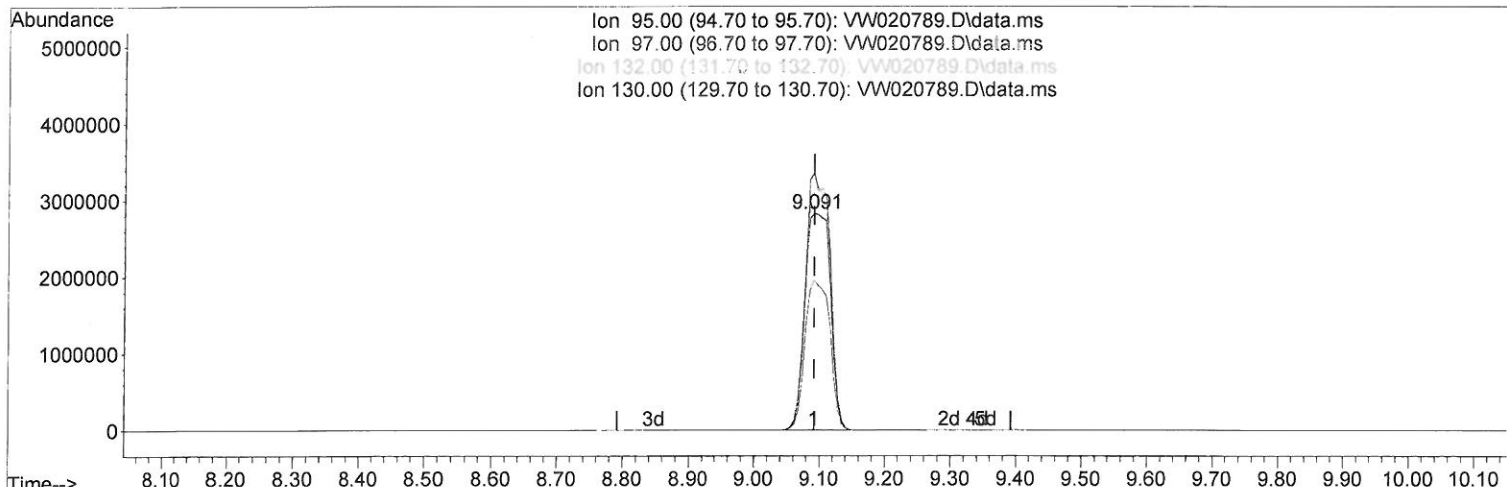

TIC: VW020789.D\data.ms

(34) Trichloroethene (T)

9.091min (-0.000) 4684.55 ug/L m

response 7670268

Ion	Exp%	Act%
95.00	100.00	100.00
97.00	67.10	69.19
132.00	93.50	109.85
130.00	99.10	118.52

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110621\
 Data File : VW020789.D
 Acq On : 05 Nov 2021 19:12
 Operator : SY/VA
 Sample : M4464-03MSD
 Misc : 6.82g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GB7K1MSD

Manual IntegrationsAPPROVED

Quant Time: Nov 08 04:54:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110621SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Nov 08 04:38:07 2021
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 11/08/2021
 Supervised By :Mahesh Dadoda 11/10/2021

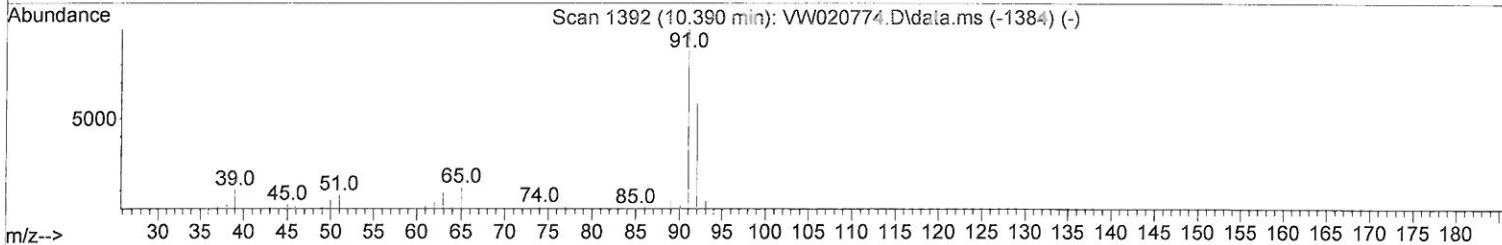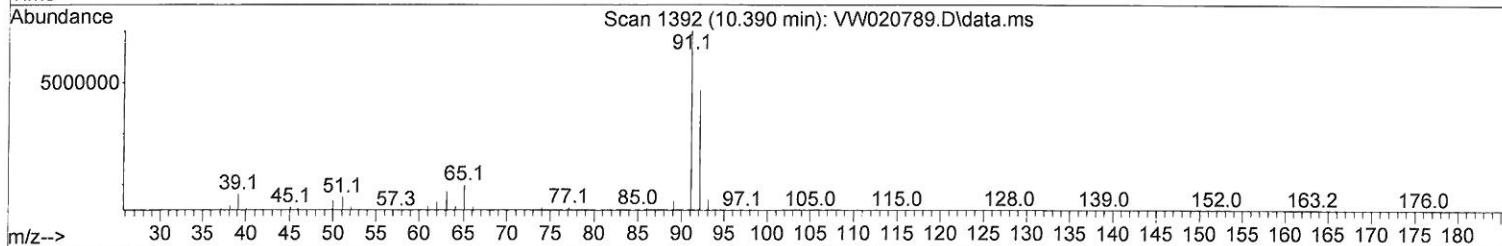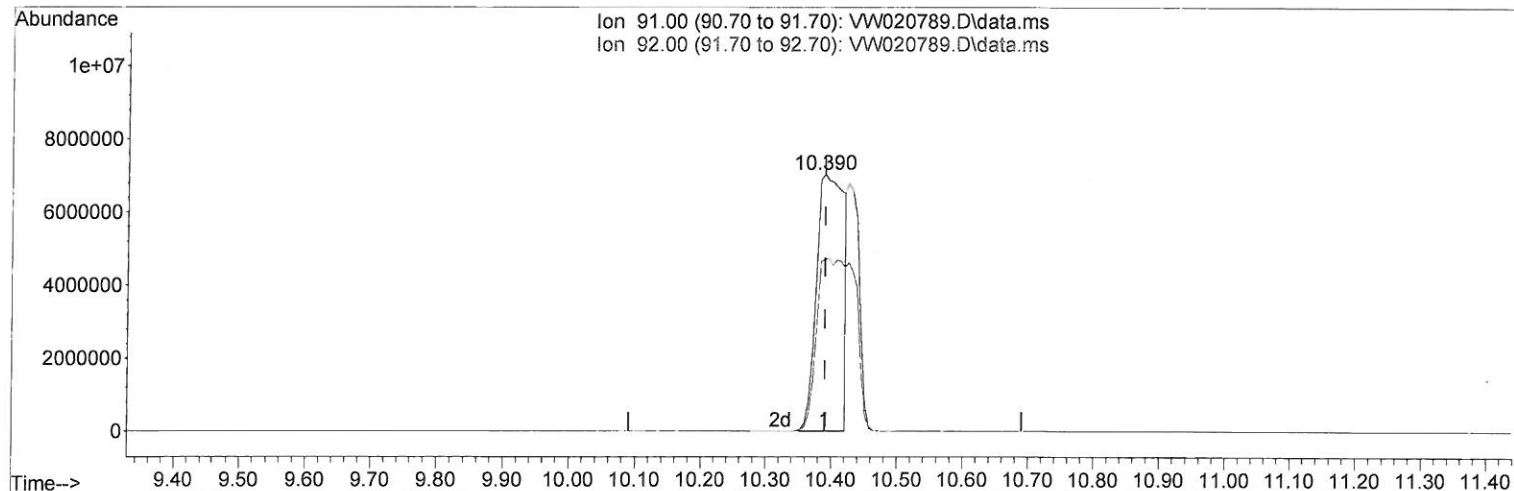

TIC: VW020789.D\data.ms

(42) Toluene (T)

10.390min (-0.000) 3054.68 ug/L

response 20205741

Ion	Exp%	Act%
91.00	100.00	100.00
92.00	59.60	66.84
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110621\
 Data File : VW020789.D
 Acq On : 05 Nov 2021 19:12
 Operator : SY/VA
 Sample : M4464-03MSD
 Misc : 6.82g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GB7K1MSD

Manual IntegrationsAPPROVED

Quant Time: Nov 08 04:54:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110621SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Nov 08 04:38:07 2021
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 11/08/2021
 Supervised By :Mahesh Dadoda 11/10/2021

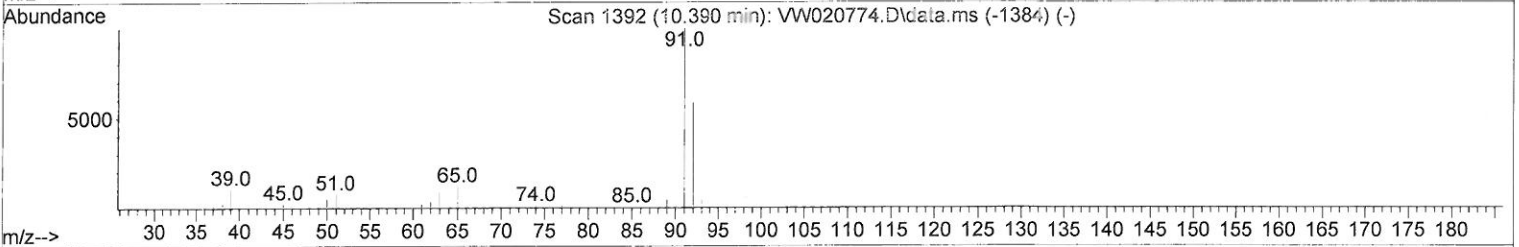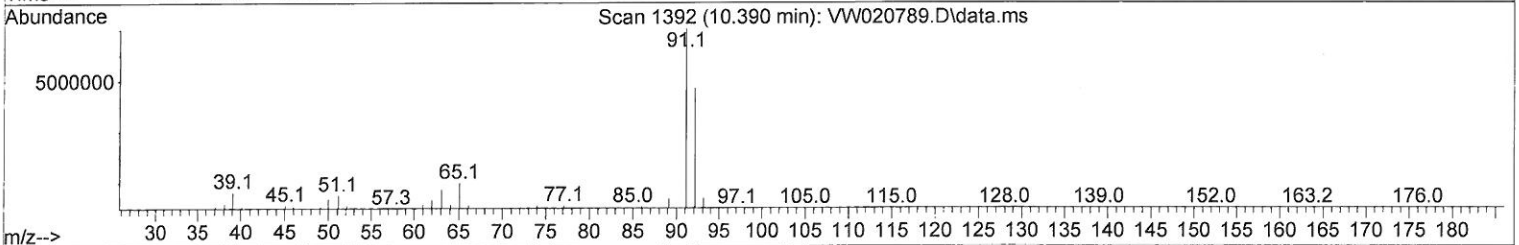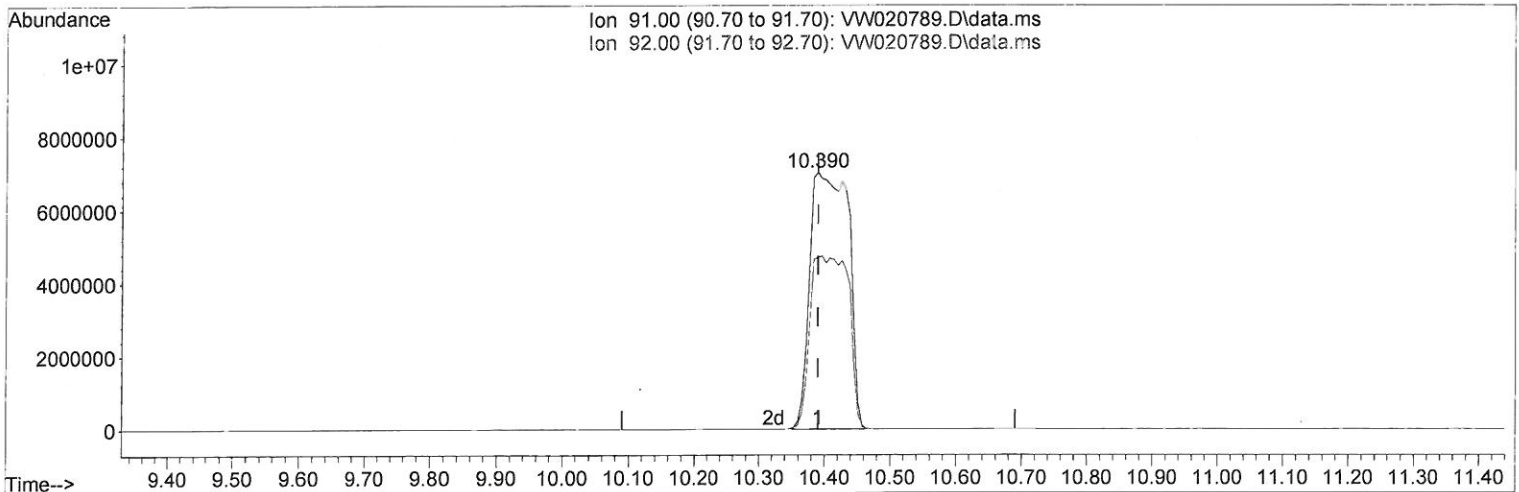

TIC: VW020789.D\data.ms

(42) Toluene (T)

10.390min (-0.000) 4327.24 ug/L m

response 28623386

Ion	Exp%	Act%
91.00	100.00	100.00
92.00	59.60	66.84
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110621\
 Data File : VW020789.D
 Acq On : 05 Nov 2021 19:12
 Operator : SY/VA
 Sample : M4464-03MSD
 Misc : 6.82g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GB7K1MSD

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 11/08/2021
 Supervised By :Mahesh Dadoda 11/10/2021

Quant Time: Nov 08 04:54:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110621SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Nov 08 04:38:07 2021
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards							
1) 1,4-Difluorobenzene		8.842	114	128451	25.000	ug/L	0.00
28) Chlorobenzene-d5		11.628	117	102710	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.554	152	32637	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.349	65	31594	26.160	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 104.640%		
7) Chloroethane-d5		2.879	69	18866m	27.574	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 110.280%		
11) 1,1-Dichloroethene-d2		4.031	63	116486	45.951	ug/L	0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	= 183.800%#		
21) 2-Butanone-d5		7.104	46	29530	73.625	ug/L	0.02
Spiked Amount	50.000	Range	20 - 135	Recovery	= 147.240%#		
24) Chloroform-d		7.647	84	66582	23.328	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	= 93.320%		
26) 1,2-Dichloroethane-d4		8.305	65	40601	26.722	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	= 106.880%		
32) Benzene-d6		8.275	84	121468	26.176	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	= 104.720%		
36) 1,2-Dichloropropane-d6		9.274	67	37860	26.351	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	= 105.400%		
41) Toluene-d8		10.335	98	105036	23.266	ug/L	0.01
Spiked Amount	25.000	Range	30 - 130	Recovery	= 93.080%		
43) trans-1,3-Dichloroprop...		10.579	79	21888	30.715	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	= 122.880%		
47) 2-Hexanone-d5		10.920	63	24539	84.413	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	= 168.820%#		
56) 1,1,2,2-Tetrachloroeth...		12.688	84	39097	32.835	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	= 131.320%#		
66) 1,2-Dichlorobenzene-d4		13.847	152	26150	25.496	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	= 102.000%		
Target Compounds							Qvalue
2) Dichlorodifluoromethane		2.007	85	24910	47.559	ug/L	99
3) Chloromethane		2.209	50	36110	26.348	ug/L	100
5) Vinyl chloride		2.355	62	296826	150.154	ug/L	96
6) Bromomethane		2.769	94	26811	26.207	ug/L	94
8) Chloroethane		2.916	64	28560	39.291	ug/L	96
9) Trichlorofluoromethane		3.251	101	12637	12.053	ug/L	99
10) 1,1,2-Trichloro-1,2,2-...		4.056	101	446888	259.153	ug/L	91
12) 1,1-Dichloroethene		4.038	96	150717	91.712	ug/L #	76
13) Acetone		4.123	43	886904	2406.454	ug/L	94
14) Carbon disulfide		4.385	76	155809	31.410	ug/L	99
15) Methyl Acetate		4.665	43	23030	32.936	ug/L	97
16) Methylene chloride		4.915	84	42873	22.540	ug/L	89
17) trans-1,2-Dichloroethene		5.428	96	97953	56.073	ug/L	89
18) Methyl tert-butyl Ether		5.428	73	61904	25.043	ug/L #	79
19) 1,1-Dichloroethane		6.214	63	1747860	577.714	ug/L	99
20) cis-1,2-Dichloroethene		7.153	96	13170065	7151.932	ug/L #	62
22) 2-Butanone		7.189	43	93519	188.992	ug/L #	1
23) Bromochloromethane		7.513	128	21507	25.309	ug/L #	71
25) Chloroform		7.677	83	74666	23.706	ug/L	98

11/10/21 Sy

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110621\
 Data File : VW020789.D
 Acq On : 05 Nov 2021 19:12
 Operator : SY/VA
 Sample : M4464-03MSD
 Misc : 6.82g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GB7K1MSD

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 11/08/2021
 Supervised By :Mahesh Dadoda 11/10/2021

Quant Time: Nov 08 04:54:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110621SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Nov 08 04:38:07 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
27) 1,2-Dichloroethane	8.403	62	83059	40.735	ug/L	97
29) Cyclohexane	7.958	56	83153	31.030	ug/L	92
30) 1,1,1-Trichloroethane	7.872	97	226927	92.972	ug/L	95
31) Carbon tetrachloride	8.067	117	53069	22.848	ug/L	100
33) Benzene	8.323	78	221388	35.991	ug/L	100
34) Trichloroethene	9.091	95	7670268m	4684.546	ug/L	
35) Methylcyclohexane	9.335	83	42297	14.803	ug/L	90
37) 1,2-Dichloropropane	9.372	63	38396	26.364	ug/L #	98
38) Bromodichloromethane	9.646	83	56496	27.712	ug/L	99
39) cis-1,3-Dichloropropene	10.073	75	65427	27.604	ug/L	99
40) 4-Methyl-2-pentanone	10.232	43	236758	248.740	ug/L #	95
42) Toluene	10.390	91	28623386m	4327.243	ug/L	
44) trans-1,3-Dichloropropene	10.610	75	65307	30.461	ug/L	100
45) 1,1,2-Trichloroethane	10.786	97	38685	35.792	ug/L	94
46) Tetrachloroethene	10.866	164	137579	93.679	ug/L	95
48) 2-Hexanone	10.969	43	65910	94.832	ug/L	90
49) Dibromochloromethane	11.128	129	43449	29.437	ug/L	95
50) 1,2-Dibromoethane	11.237	107	34636	31.605	ug/L #	99
51) Chlorobenzene	11.658	112	95799	22.454	ug/L	96
52) Ethylbenzene	11.731	91	426132	57.499	ug/L	98
53) m,p-Xylene	11.835	106	465267	156.689	ug/L	90
54) o-Xylene	12.164	106	197266	70.132	ug/L	96
55) Styrene	12.176	104	101558	21.238	ug/L	88
57) 1,1,2,2-Tetrachloroethane	12.713	83	40138	31.686	ug/L #	98
59) Bromoform	12.347	173	26761	48.477	ug/L #	97
60) Isopropylbenzene	12.463	105	132751	29.511	ug/L	96
61) 1,2,3-Trichloropropane	12.768	75	30376	56.319	ug/L	93
62) 1,3,5-Trimethylbenzene	12.938	105	105707	27.347	ug/L	96
63) 1,2,4-Trimethylbenzene	13.249	105	195910	51.020	ug/L	90
64) 1,3-Dichlorobenzene	13.499	146	46351	22.224	ug/L	97
65) 1,4-Dichlorobenzene	13.579	146	47209	22.723	ug/L	92
67) 1,2-Dichlorobenzene	13.871	146	60767	32.983	ug/L	94
68) 1,2-Dibromo-3-chloropr...	14.481	75	7213	54.708	ug/L #	73
69) 1,3,5-Trichlorobenzene	14.627	180	20606	12.447	ug/L	99
70) 1,2,4-trichlorobenzene	15.127	180	15194	11.009	ug/L	99
71) Naphthalene	15.359	128	53871	23.093	ug/L	100
72) 1,2,3-Trichlorobenzene	15.554	180	13627	11.619	ug/L	94

11/10/21 Sy

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110621\
 Data File : VW020789.D
 Acq On : 05 Nov 2021 19:12
 Operator : SY/VA
 Sample : M4464-03MSD
 Misc : 6.82g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GB7K1MSD

Manual IntegrationsAPPROVED

Quant Time: Nov 08 04:54:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110621SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Nov 08 04:38:07 2021
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 11/08/2021
 Supervised By :Mahesh Dadoda 11/10/2021

