

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110621\
 Data File : VW020783.D
 Acq On : 05 Nov 2021 16:47
 Operator : SY/VA
 Sample : M4511-01
 Misc : 5.19g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4263

Quant Time: Nov 08 04:53:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110621SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Nov 08 04:38:07 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	192126	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117	170639	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	87800	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	47164	26.109	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	104.440%
7) Chloroethane-d5	2.879	69	25833	25.243	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	100.960%
11) 1,1-Dichloroethene-d2	4.013	63	58909	15.537	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	62.160%
21) 2-Butanone-d5	7.080	46	22658	37.769	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	75.540%
24) Chloroform-d	7.647	84	91316	21.391	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	85.560%
26) 1,2-Dichloroethane-d4	8.305	65	49390	21.733	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	86.920%
32) Benzene-d6	8.275	84	186019	24.128	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	96.520%
36) 1,2-Dichloropropane-d6	9.274	67	54171	22.695	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	90.760%
41) Toluene-d8	10.323	98	180727	24.095	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	96.400%
43) trans-1,3-Dichloroprop...	10.579	79	25633	21.651	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.600%
47) 2-Hexanone-d5	10.920	63	19236	39.829	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	79.660%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	38503	19.464	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	77.840%
66) 1,2-Dichlorobenzene-d4	13.853	152	60664	21.986	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	87.960%
Target Compounds					Qvalue	
13) Acetone	4.129	43	2713	4.922	ug/L	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110621\
Data File : VW020783.D
Acq On : 05 Nov 2021 16:47
Operator : SY/VA
Sample : M4511-01
Misc : 5.19g/10.0mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4263

Quant Time: Nov 08 04:53:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110621SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Nov 08 04:38:07 2021
Response via : Initial Calibration

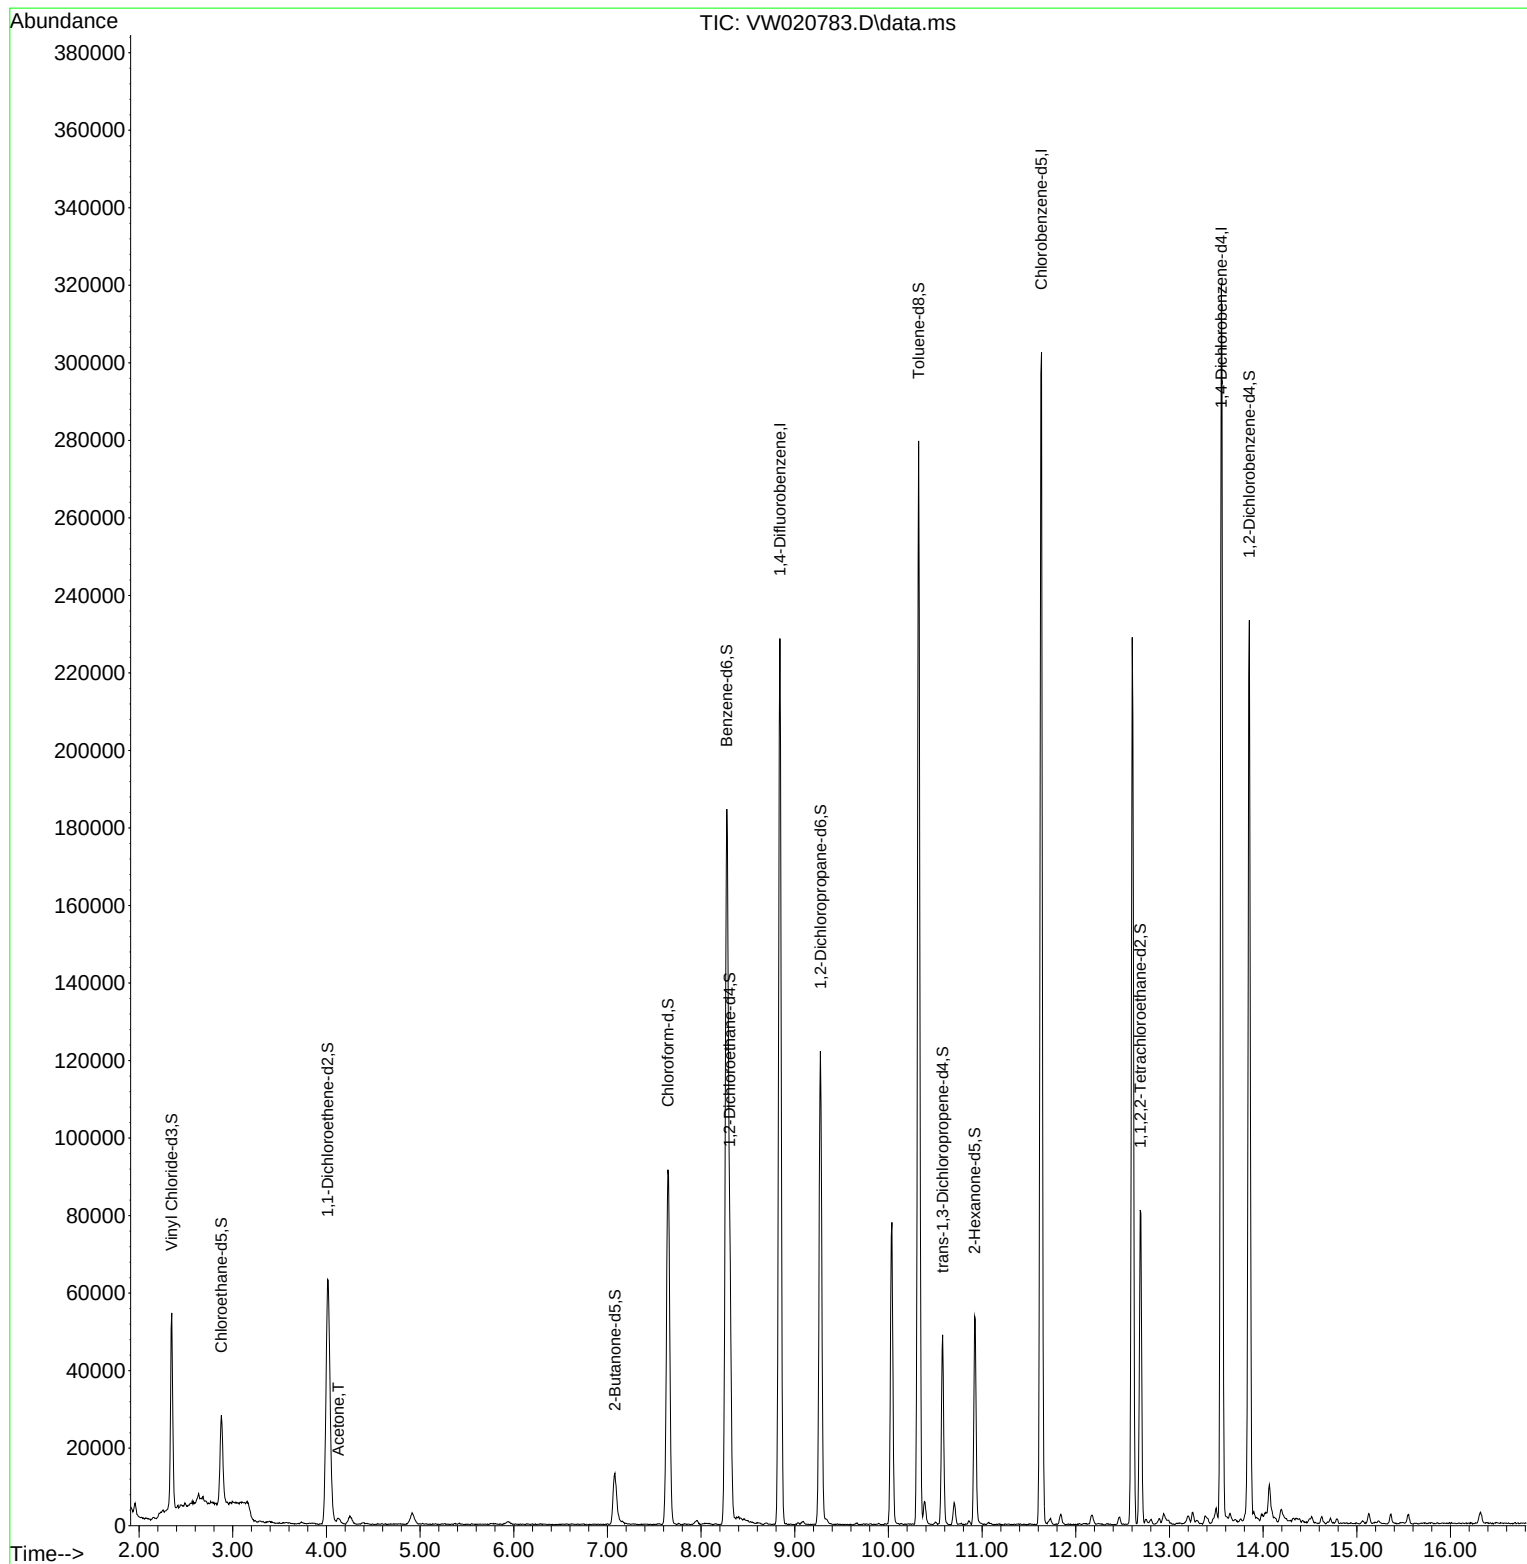

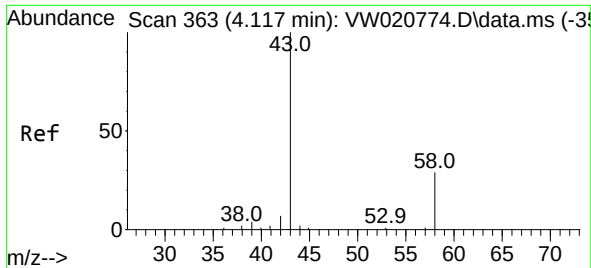

#13

Acetone

Concen: 4.922 ug/L

RT: 4.129 min Scan# 30

Delta R.T. 0.006 min

Lab File: VW020783.D


Acq: 05 Nov 2021 16:47

Instrument :

MSVOA_W

ClientSampleId :

A4263

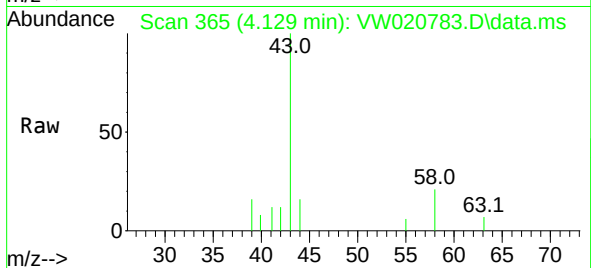

Tgt Ion: 43 Resp: 2713

Ion Ratio Lower Upper

43 100

58 15.0 0.0 52.8

