

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110621\
 Data File : VW020784.D
 Acq On : 05 Nov 2021 17:12
 Operator : SY/VA
 Sample : M4511-05
 Misc : 5.52g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4269

Quant Time: Nov 08 04:53:38 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110621SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Nov 08 04:38:07 2021
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		8.841	114	119131	25.000	ug/L	# 0.00
28) Chlorobenzene-d5		11.628	117	108088	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.560	152	57819	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.349	65	28742	25.660	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	102.640%	
7) Chloroethane-d5		2.879	69	16766	26.422	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	105.680%	
11) 1,1-Dichloroethene-d2		4.013	63	39319	16.724	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.880%	
21) 2-Butanone-d5		7.074	46	16386	44.050	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	88.100%	
24) Chloroform-d		7.653	84	60039	22.681	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	90.720%	
26) 1,2-Dichloroethane-d4		8.305	65	33747	23.948	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.800%	
32) Benzene-d6		8.274	84	120622	24.700	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	98.800%	
36) 1,2-Dichloropropane-d6		9.274	67	36110	23.883	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.520%	
41) Toluene-d8		10.323	98	116787	24.581	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	98.320%	
43) trans-1,3-Dichloroprop...		10.579	79	17131	22.844	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	91.360%	
47) 2-Hexanone-d5		10.920	63	13667	44.674	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.340%	
56) 1,1,2,2-Tetrachloroeth...		12.694	84	28558	22.791	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	91.160%	
66) 1,2-Dichlorobenzene-d4		13.853	152	44227	24.340	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.360%	
Target Compounds							
13) Acetone		4.129	43	1992	5.828	ug/L	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110621\
Data File : VW020784.D
Acq On : 05 Nov 2021 17:12
Operator : SY/VA
Sample : M4511-05
Misc : 5.52g/10.0mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4269

Quant Time: Nov 08 04:53:38 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110621SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Nov 08 04:38:07 2021
Response via : Initial Calibration

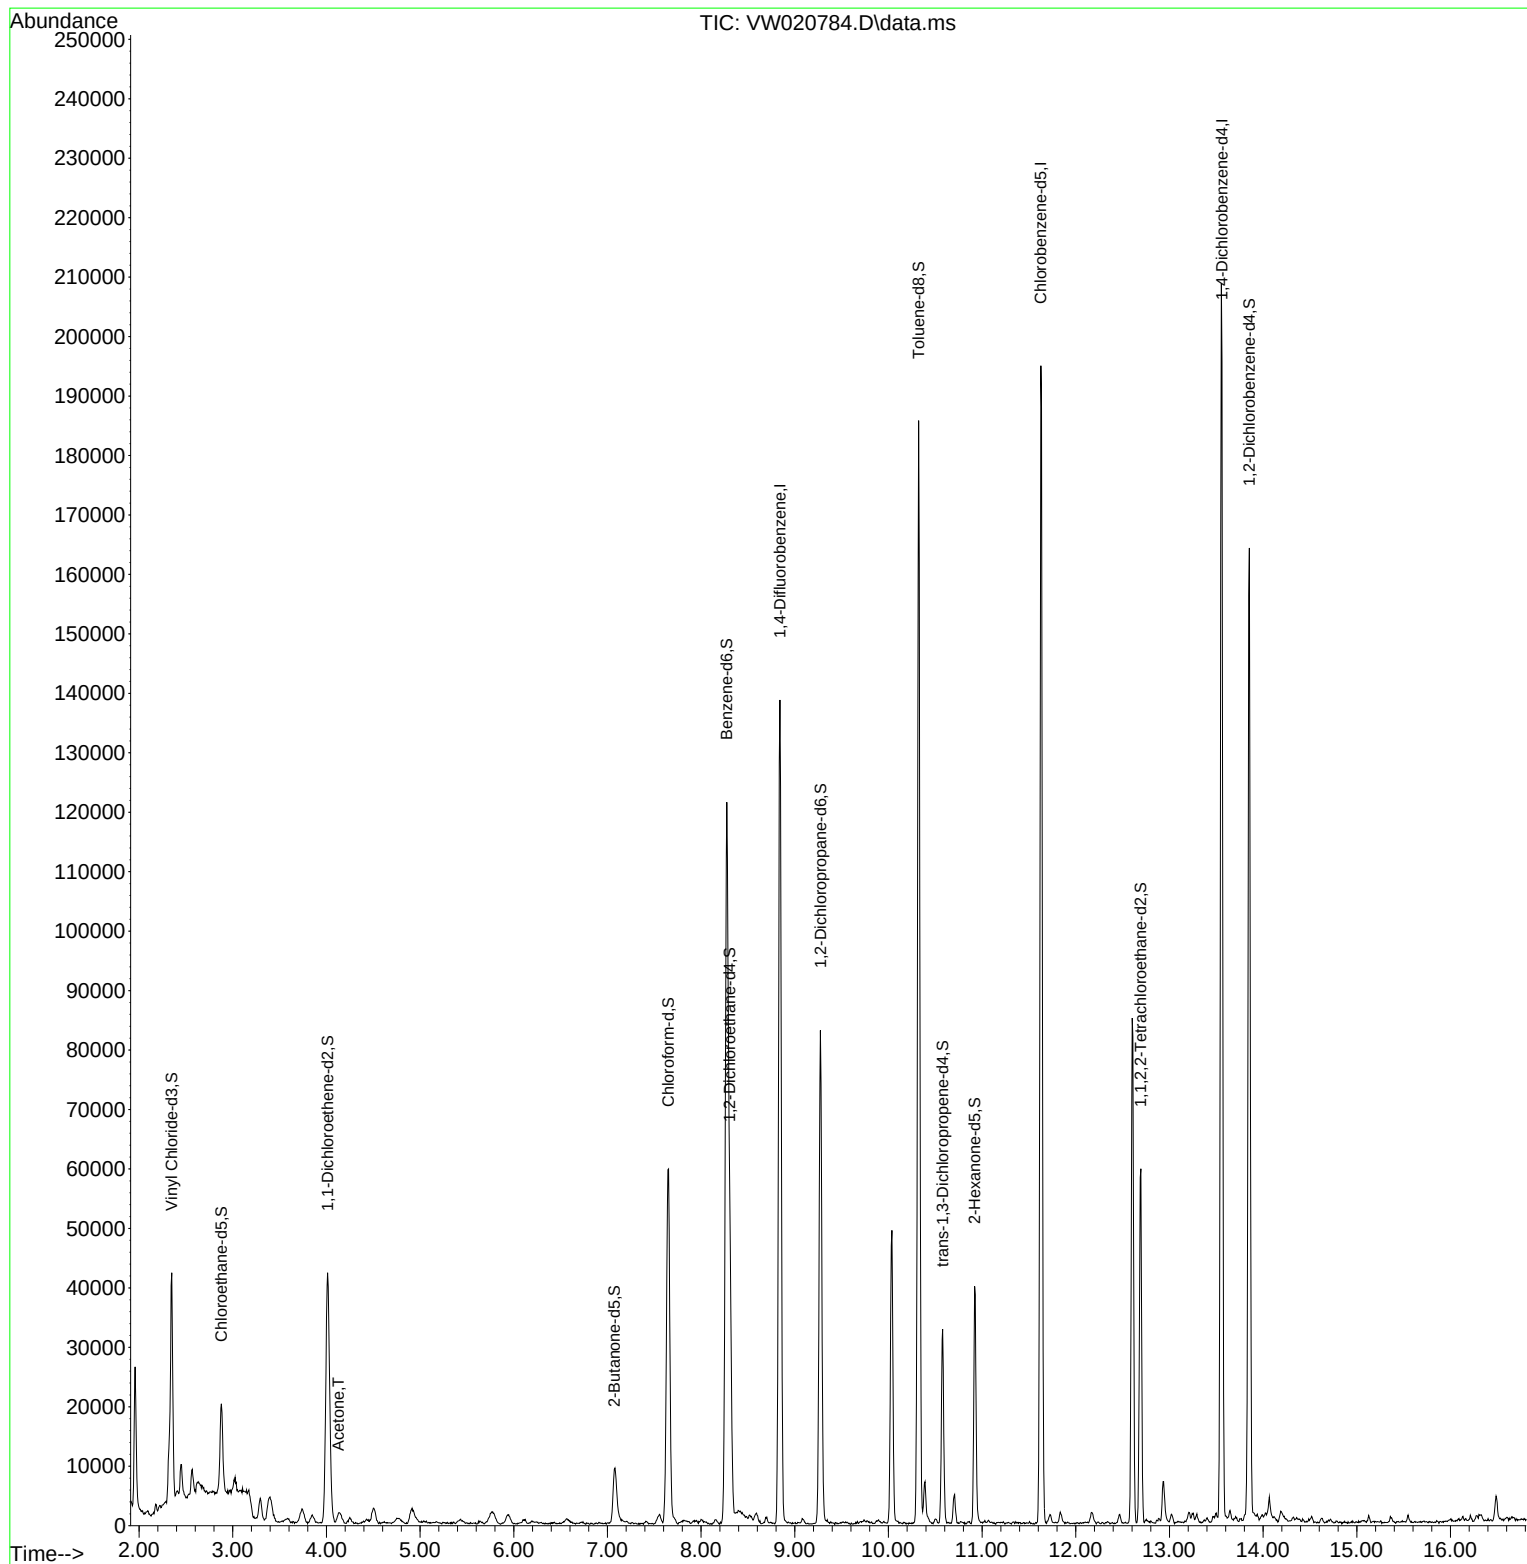

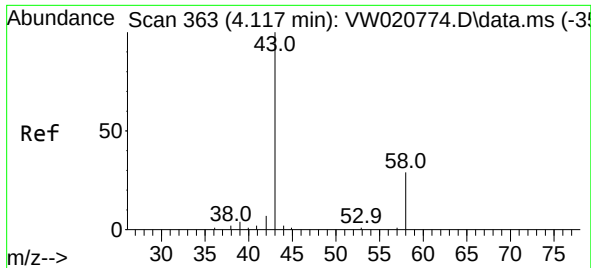

#13

Acetone

Concen: 5.828 ug/L

RT: 4.129 min Scan# 30

Delta R.T. 0.006 min

Lab File: VW020784.D


Acq: 05 Nov 2021 17:12

Instrument :

MSVOA_W

ClientSampleId :

A4269

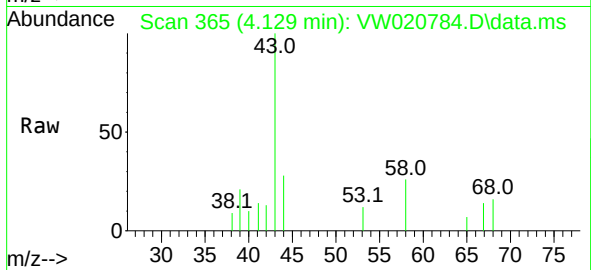

Tgt Ion: 43 Resp: 1992

Ion Ratio Lower Upper

43 100

58 28.8 0.0 52.8

