

Data File : VW013929.D
Acq On : 07 Nov 2019 13:51
Operator : SY/VA
Sample : VW1107SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK21

Quant Time: Nov 08 00:51:58 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110119S.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 08 00:49:30 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	309756	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	304283	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	172438	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	90479	18.77	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.08%
7) Chloroethane-d5	2.89	69	79831	20.73	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.92%
10) 1,1-Dichloroethene-d2	4.02	63	141411	14.40	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.60%
20) 2-Butanone-d5	7.07	46	77874	44.90	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.80%
24) Chloroform-d	7.65	84	214692	22.00	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.00%
26) 1,2-Dichloroethane-d4	8.31	65	119092	22.67	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.68%
29) Benzene-d6	8.27	84	442658	21.72	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	86.88%
33) 1,2-Dichloropropane-d6	9.27	67	138911	22.51	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	90.04%
37) Toluene-d8	10.32	98	404872	20.94	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	83.76%
38) trans-1,3-Dichloropropene-	10.58	79	60744	21.56	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.24%
39) 2-Hexanone-d5	10.92	63	64206	45.81	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.62%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	127252	23.31	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	93.24%
61) 1,2-Dichlorobenzene-d4	13.85	152	161371	23.65	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	94.60%


Target Compounds					Qvalue
59) 1,2,3-Trichloropropane	13.55	75	18240	4.455 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VW013929.D
Acq On : 07 Nov 2019 13:51
Operator : SY/VA
Sample : VW1107SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK21

Quant Time: Nov 08 00:51:58 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110119S.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 08 00:49:30 2019
Response via : Initial Calibration

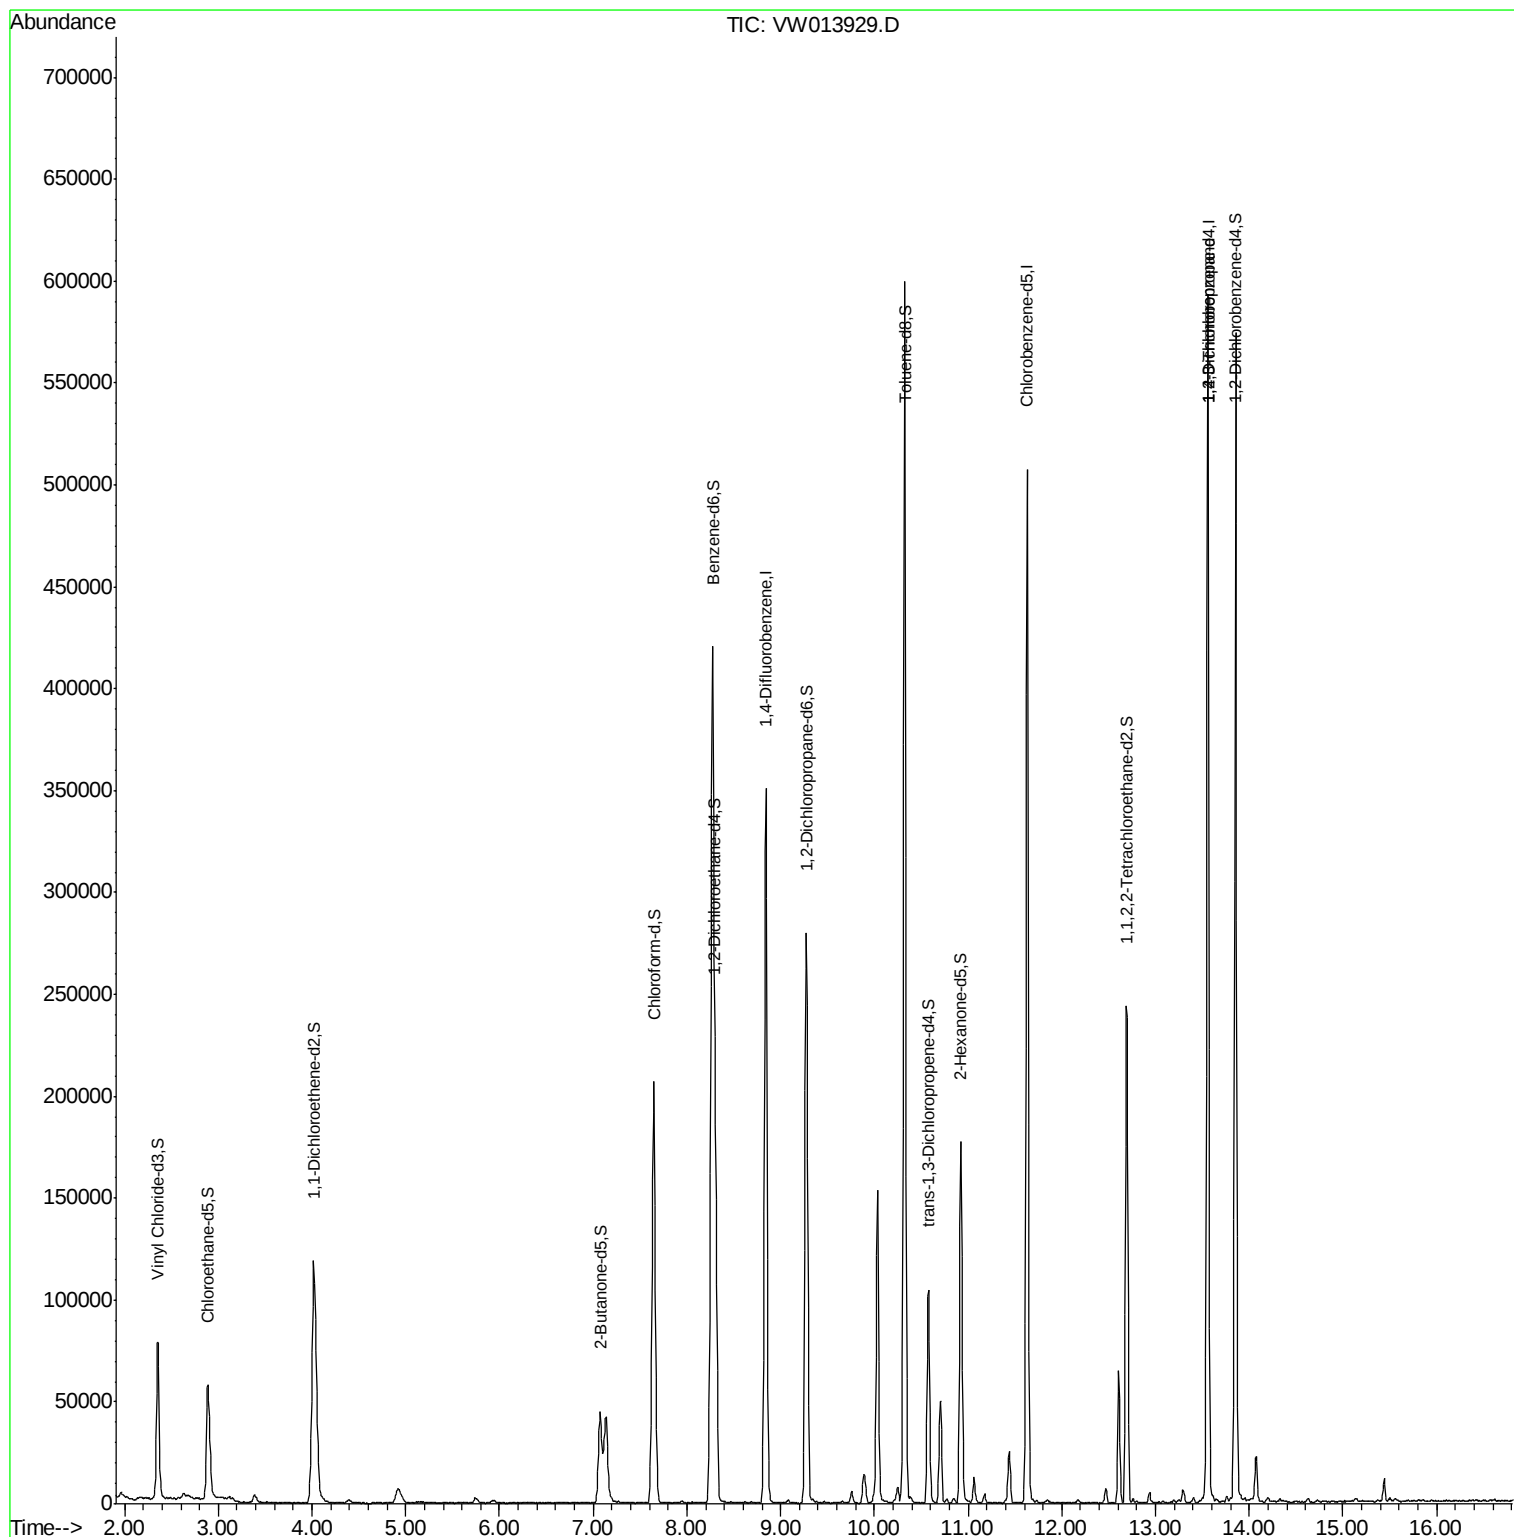

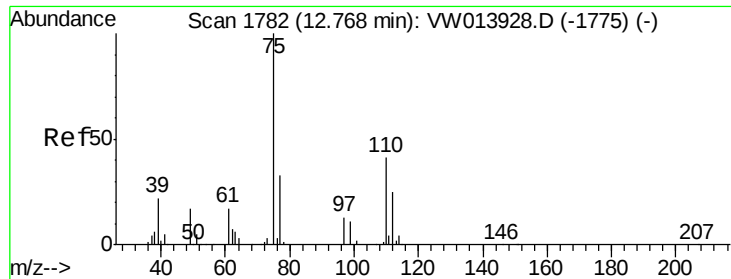

#59

1,2,3-Trichloropropane

Concen: 4.455 ug/L

RT: 13.55 min Scan# 1911

Delta R.T. 0.79 min

Lab File: VW013929.D

Acq: 07 Nov 2019 13:51

Instrument :

MSVOA_W

ClientSampleId :

VBLK21

Tgt Ion: 75 Resp: 18240

Ion Ratio Lower Upper

75 100

77 32.8 25.9 38.9

