

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110824\
 Data File : VW030961.D
 Acq On : 08 Nov 2024 10:59
 Operator : SY/MD
 Sample : VW1108SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 08 22:05:15 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Nov 08 22:04:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	444963	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	429907	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	191735	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	113459	15.547	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	62.200%
7) Chloroethane-d5	2.893	69	96809	17.296	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	69.200%
11) 1,1-Dichloroethene-d2	4.021	65	56479	18.756	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	75.040%
21) 2-Butanone-d5	7.081	46	61884	51.529	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.060%
24) Chloroform-d	7.648	84	288388	21.985	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	87.920%
26) 1,2-Dichloroethane-d4	8.301	65	149071	22.856	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.440%
32) Benzene-d6	8.270	84	555566	20.802	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	83.200%
36) 1,2-Dichloropropane-d6	9.270	67	169931	21.583	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	86.320%
41) Toluene-d8	10.325	98	504005	21.039	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	84.160%
43) trans-1,3-Dichloroprop...	10.575	79	66410	20.809	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.240%
47) 2-Hexanone-d5	10.922	63	51673	50.641	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.280%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	133792	24.391	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	97.560%
66) 1,2-Dichlorobenzene-d4	13.848	152	170241	24.375	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.520%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	4575	0.442	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110824\
Data File : VW030961.D
Acq On : 08 Nov 2024 10:59
Operator : SY/MD
Sample : VW1108SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Nov 08 22:05:15 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Nov 08 22:04:34 2024
Response via : Initial Calibration

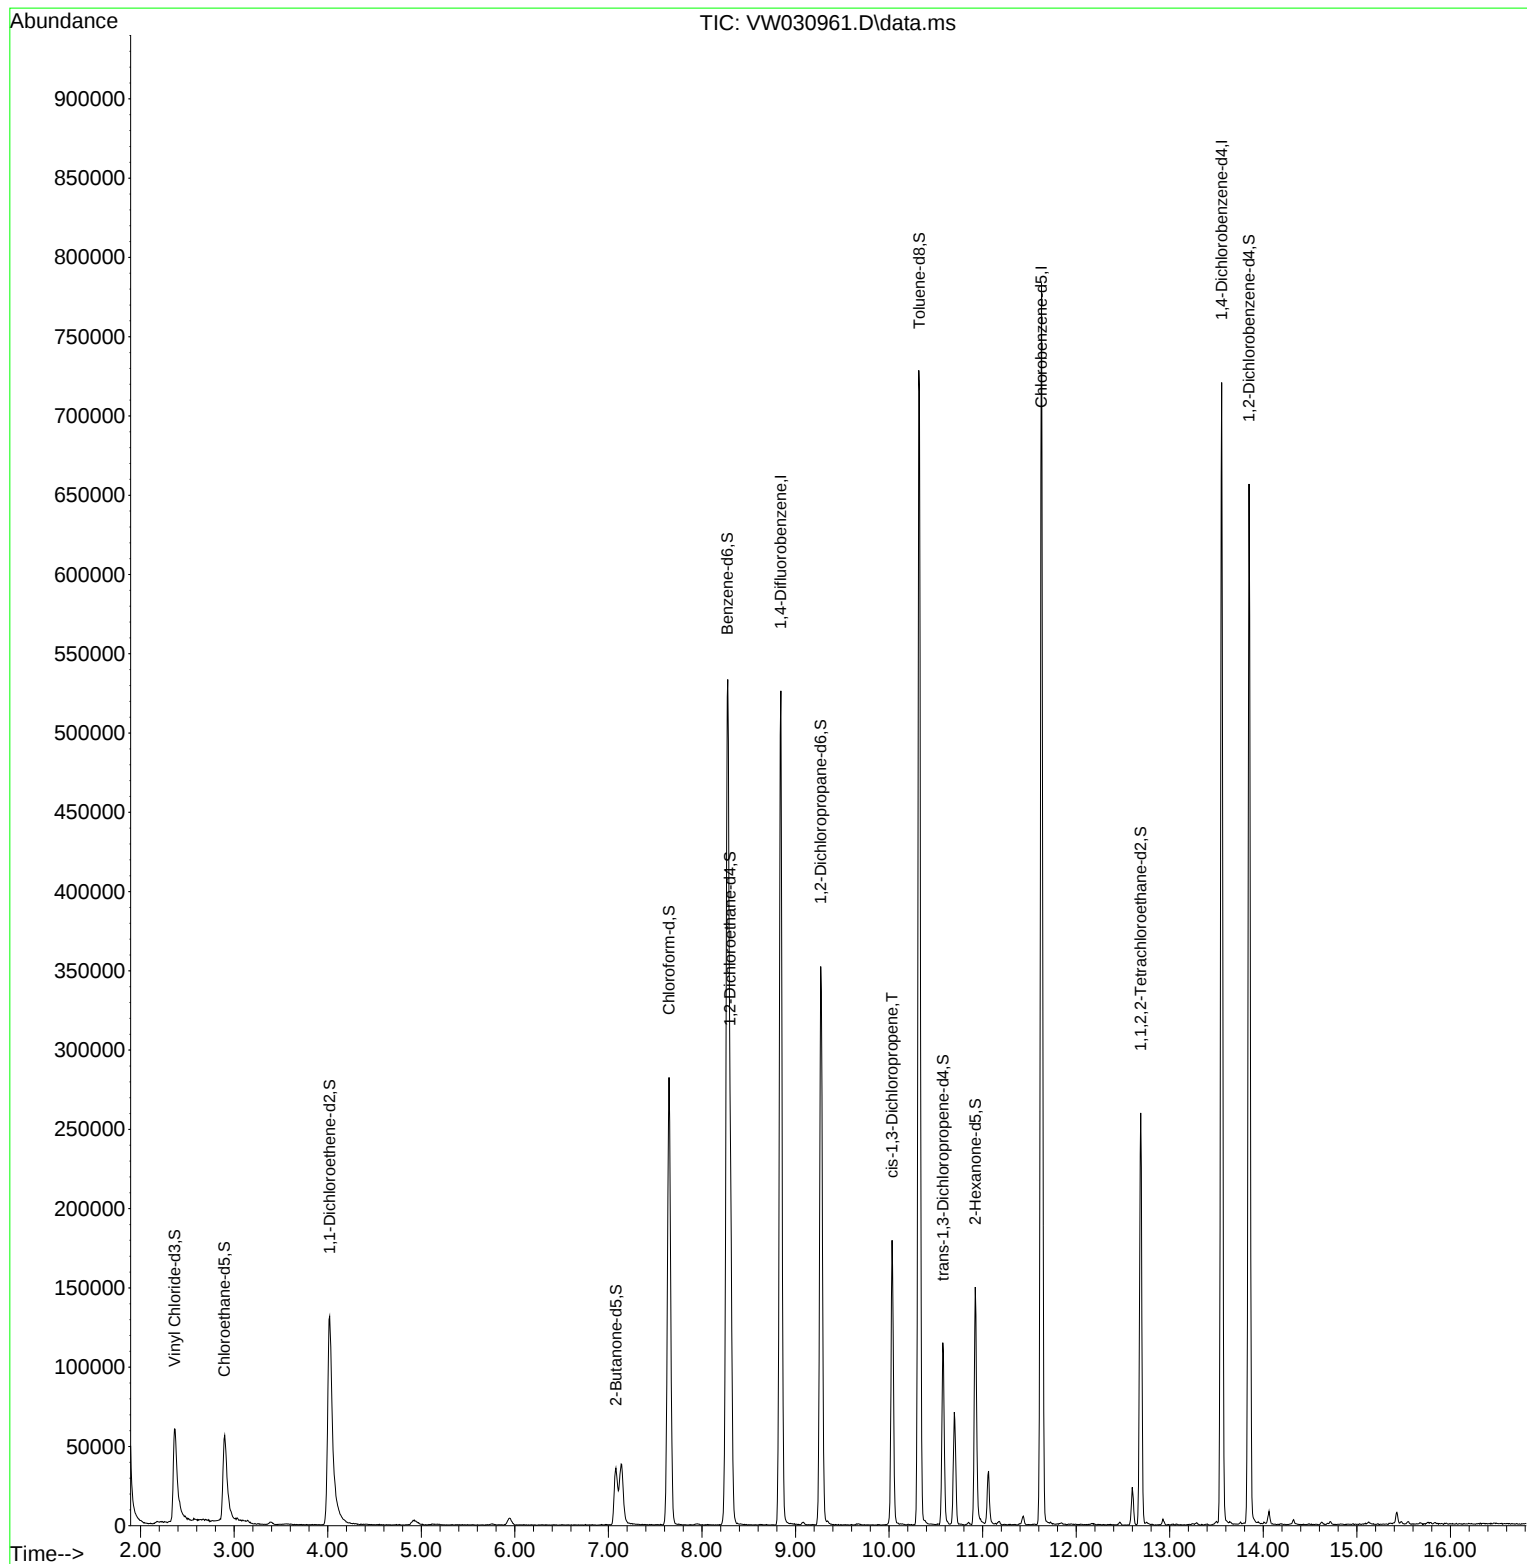

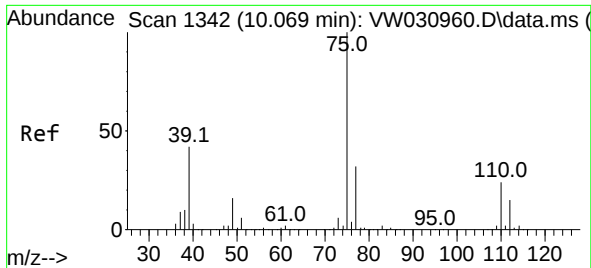

#39
 cis-1,3-Dichloropropene
 Concen: 0.442 ug/L
 RT: 10.032 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW030961.D
 Acq: 08 Nov 2024 10:59

Instrument :
 MSVOA_W
 ClientSampleId :

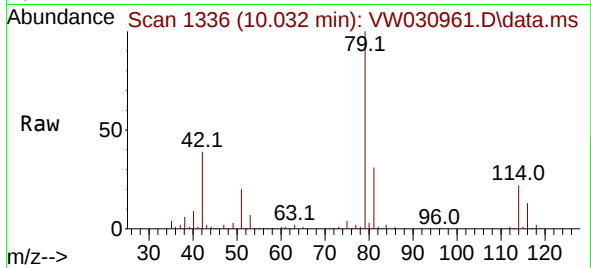

Tgt Ion: 75 Resp: 4575
 Ion Ratio Lower Upper
 75 100
 77 34.6 21.3 39.6

