

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110824\
 Data File : VW030962.D
 Acq On : 08 Nov 2024 11:31
 Operator : SY/MD
 Sample : P4724-12
 Misc : 6.29g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 08 22:05:28 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Nov 08 22:04:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	404652	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	392317	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	178153	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	99803	15.038	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	60.160%
7) Chloroethane-d5	2.899	69	80950	15.904	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	63.600%
11) 1,1-Dichloroethene-d2	4.021	65	46791	17.086	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.360%
21) 2-Butanone-d5	7.075	46	61408	56.226	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	112.460%
24) Chloroform-d	7.648	84	240286	20.143	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	80.560%
26) 1,2-Dichloroethane-d4	8.301	65	129267	21.794	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	87.160%
32) Benzene-d6	8.270	84	468080	19.205	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	76.840%
36) 1,2-Dichloropropane-d6	9.270	67	144750	20.146	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	80.600%
41) Toluene-d8	10.319	98	412701	18.878	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	75.520%
43) trans-1,3-Dichloroprop...	10.575	79	56747	19.485	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	77.920%
47) 2-Hexanone-d5	10.922	63	51296	55.088	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	110.180%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	124234	24.818	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	99.280%
66) 1,2-Dichlorobenzene-d4	13.848	152	144466	22.262	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	89.040%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	3417	0.361	ug/L	# 49


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110824\
Data File : VW030962.D
Acq On : 08 Nov 2024 11:31
Operator : SY/MD
Sample : P4724-12
Misc : 6.29g/10mL/MSVOA_W/SOIL/B
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Nov 08 22:05:28 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Nov 08 22:04:34 2024
Response via : Initial Calibration

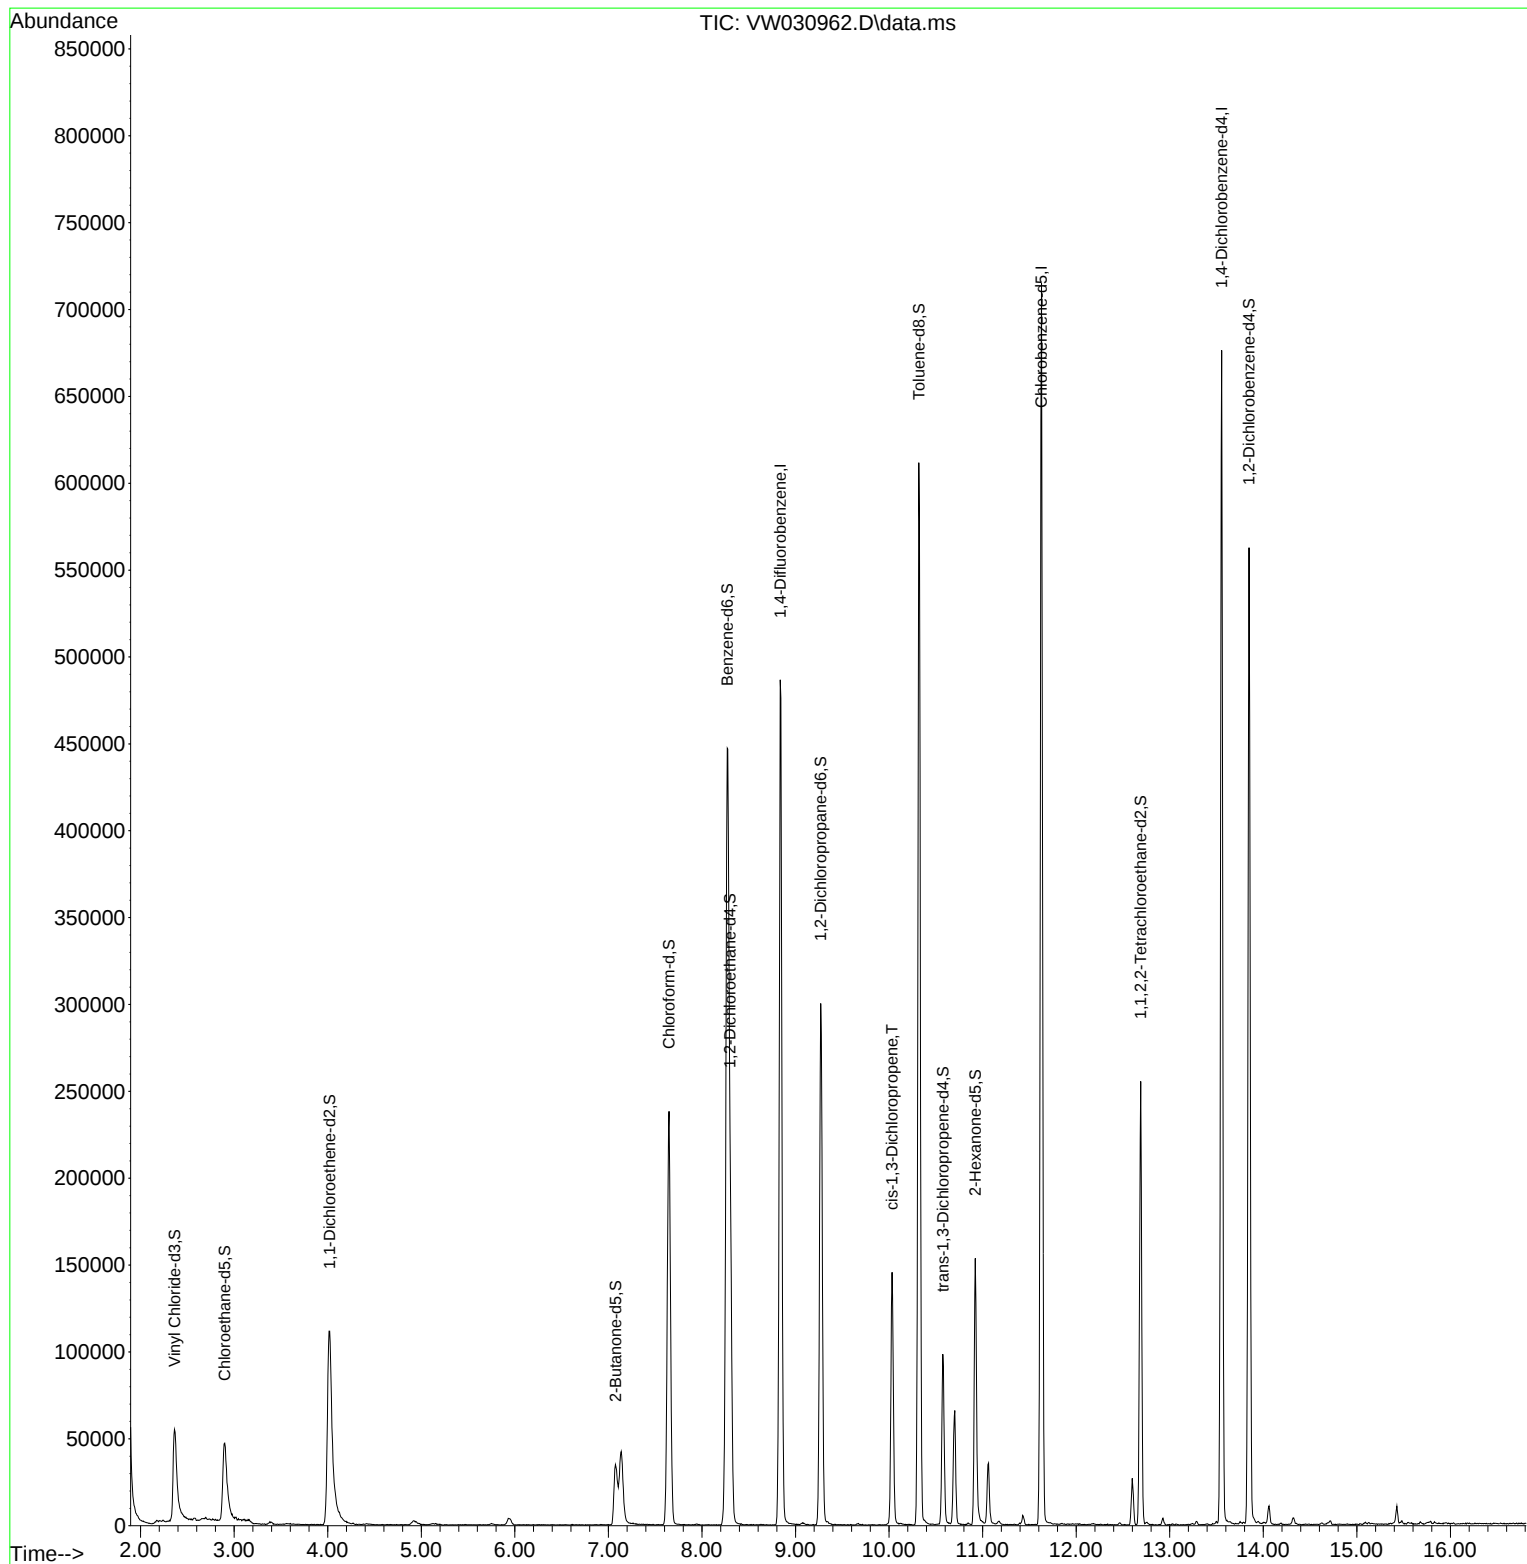

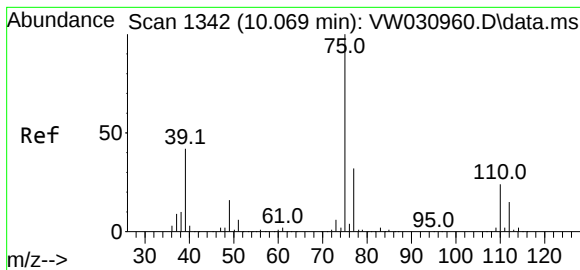

#39
 cis-1,3-Dichloropropene
 Concen: 0.361 ug/L
 RT: 10.032 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW030962.D
 Acq: 08 Nov 2024 11:31

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 3417
 Ion Ratio Lower Upper
 75 100
 77 58.2 21.3 39.6#

