

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110824\
 Data File : VW030970.D
 Acq On : 08 Nov 2024 15:15
 Operator : SY/MD
 Sample : P4751-10
 Misc : 5.74g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 08 22:07:10 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Nov 08 22:04:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	567755	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	501240	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	223261	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	153786	16.515	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	66.080%
7) Chloroethane-d5	2.905	69	117005	16.383	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	65.520%
11) 1,1-Dichloroethene-d2	4.027	65	68520	17.833	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	71.320%
21) 2-Butanone-d5	7.081	46	83586	54.547	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	109.100%
24) Chloroform-d	7.648	84	323753	19.343	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	77.360%
26) 1,2-Dichloroethane-d4	8.490	65	46	0.006	ug/L	0.19
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.040%#
32) Benzene-d6	8.276	84	622060	19.977	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	79.920%
36) 1,2-Dichloropropane-d6	9.270	67	197234	21.486	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	85.960%
41) Toluene-d8	10.325	98	539989	19.333	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	77.320%
43) trans-1,3-Dichloroprop...	10.575	79	77367	20.792	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.160%
47) 2-Hexanone-d5	10.922	63	68004	57.161	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	114.320%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	170076	26.593	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	106.360%
66) 1,2-Dichlorobenzene-d4	13.848	152	182638	22.458	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	89.840%
Target Compounds						
39) cis-1,3-Dichloropropene	10.032	75	5356	0.443	ug/L	Qvalue # 75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110824\
Data File : VW030970.D
Acq On : 08 Nov 2024 15:15
Operator : SY/MD
Sample : P4751-10
Misc : 5.74g/10mL/MSVOA_W/SOIL/B
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Nov 08 22:07:10 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Nov 08 22:04:34 2024
Response via : Initial Calibration

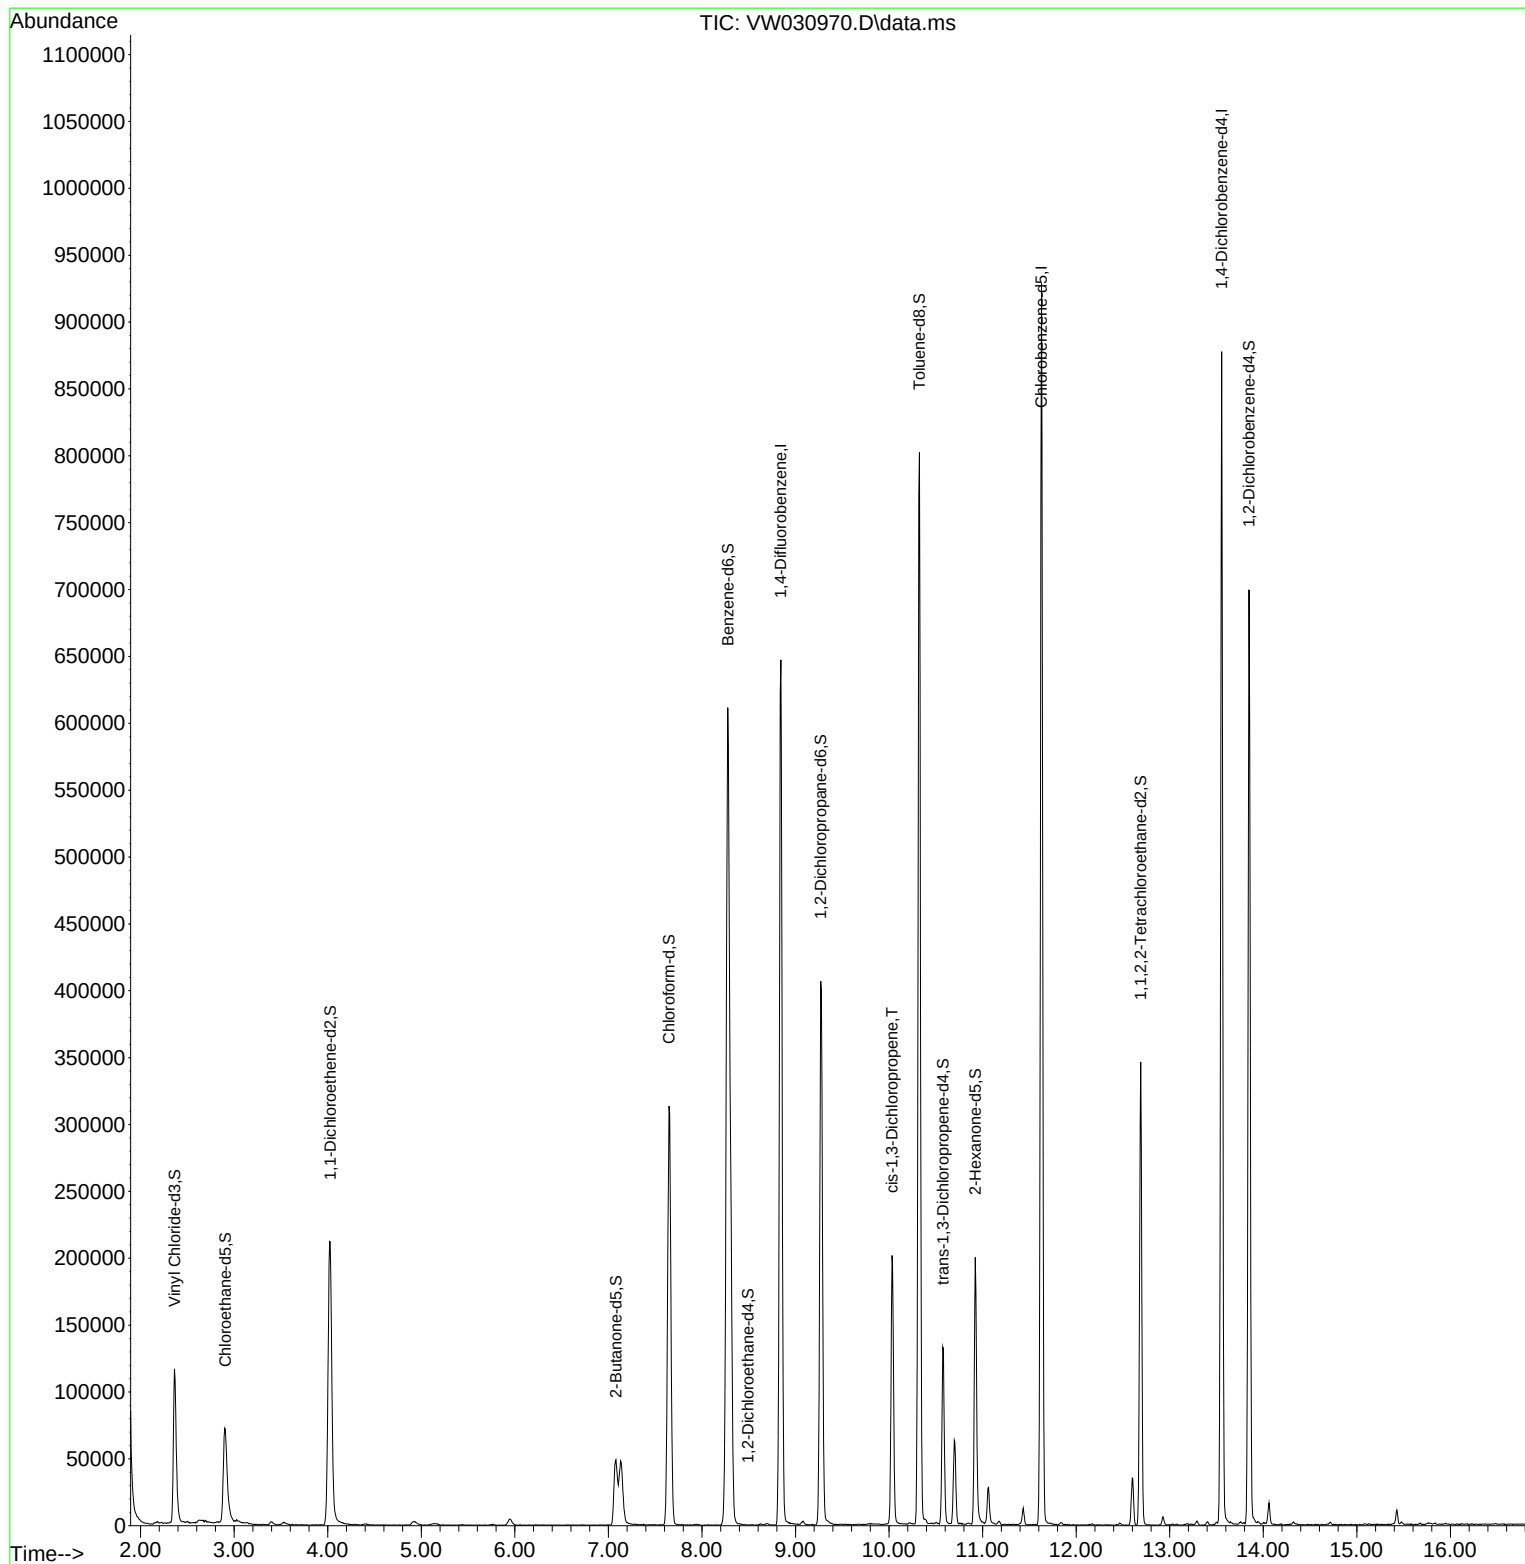

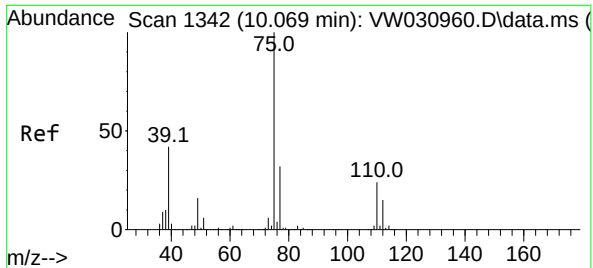

#39
 cis-1,3-Dichloropropene
 Concen: 0.443 ug/L
 RT: 10.032 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW030970.D
 Acq: 08 Nov 2024 15:15

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 5356
 Ion Ratio Lower Upper
 75 100
 77 44.3 21.3 39.6#

